

Emergence and Spread of *Chlamydia trachomatis* Variant, Sweden

Björn Herrmann, Anna Törner, Nicola Low, Markus Klint, Anders Nilsson, Inga Velicko, Thomas Söderblom, and Anders Blaxhult

A variant of *Chlamydia trachomatis* that had escaped detection by commonly used systems was discovered in Sweden in 2006. In a nationwide study, we found that it is now prevalent across Sweden, irrespective of the detection system used. Genetic analysis by multilocus sequence typing identified a predominant variant, suggesting recent emergence.

In 2006 a new variant of *Chlamydia trachomatis* (nvCT) was discovered in Sweden (1). Because of a 377-bp deletion in the target sequence for amplification, the variant had escaped detection by 2 widely used nucleic acid amplification tests, Abbott m2000 (Abbott Laboratories, Abbott Park, IL, USA) and Cobas Amplicor/TaqMan48 (Roche Diagnostics, Basel, Switzerland) (1,2). The other test commonly used in Sweden, ProbeTec ET (Becton Dickinson [BD], Franklin Lakes, NJ, USA), detects the new variant because it uses a different DNA target sequence in the cryptic plasmid (3). The nvCT has now been reported from several of Sweden's 21 counties (Figure 1). The aim of this study was to provide a national overview of the characteristics and extent of the new chlamydia variant through examination of surveillance trends, microbiologic laboratory data, and genetic analysis of new variant strains.

The Study

We examined national surveillance data reported to the Swedish Institute for Infectious Disease Control (Smittskyddsinstitutet) about chlamydia cases detected and the number of chlamydia tests performed. Trend analysis from 2004 to 2006 included only data for the first 6 months of each year to avoid any influence of changes in detection systems; some counties introduced different detec-

tion systems in late 2006 in response to the emergence of nvCT. The statistical methods are described in the online Technical Appendix (available from <http://www.cdc.gov/EID/content/14/9/1462-Techapp.pdf>). The total number of chlamydia cases detected in Sweden in the first 6 months of 2006 was lower than that in 2005, and the proportion of tests that were positive also fell (Table 1). In 2004, the proportion of positive chlamydia tests was similar whether laboratories used Abbott/Roche or BD test systems. From 2004 to 2005, there was a relative reduction of 3.4% (95% confidence interval [CI] 5.8–1.0) in chlamydia positivity in laboratories using the Abbott or Roche methods ($p = 0.006$) but no change in the proportion of positive samples in laboratories using the BD test system (–0.4%, 95% CI –4.2 to +3.5). During the first 6 months of 2005 and 2006, the positivity rates of samples tested by Abbott or Roche systems fell further; samples tested that used the BD system remained stable. The estimated difference in proportions of chlamydia-positive samples in counties that used Abbott or Roche tests compared with counties that used the BD method was –9.5 % (95% CI –14.1 to –4.7, $p = 0.0005$), after baseline differences and county differences in testing were controlled for.

We conducted microbiologic analyses on consecutive samples that were collected from 12 counties in late 2006 and early 2007. Cases of nvCT were identified by testing specimens with additional methods using alternative se-

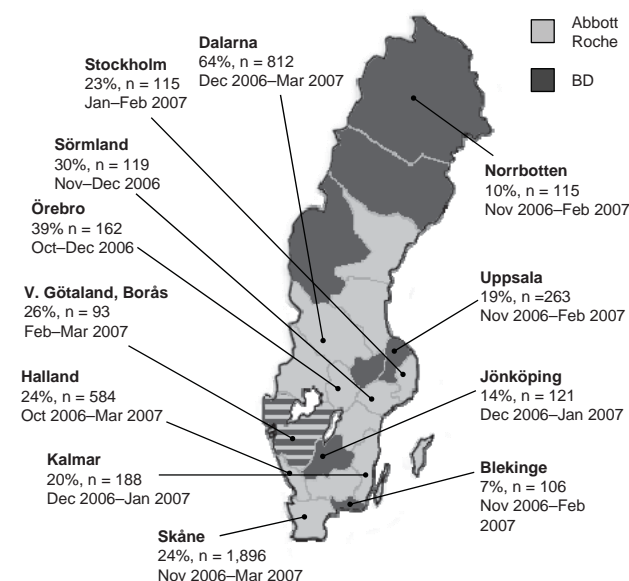


Figure 1. Map of Sweden showing proportions of the new variant of *Chlamydia trachomatis* in different counties. Light gray shading indicates counties that used Abbott or Roche test systems before the discovery of the new variant; dark gray shading indicates counties that used the Becton Dickinson (BD) system. The 1 county that used both Roche and BD assays is indicated with stripes. n, number of positive chlamydia cases analyzed. The period in which samples were collected is given for each county.

Uppsala University Hospital, Uppsala, Sweden (B. Herrmann, M. Klint, A. Nilsson); Swedish Institute for Infectious Disease Control, Solna, Sweden (A. Törner, I. Velicko, T. Söderblom, A. Blaxhult); and University of Bern, Bern, Switzerland (N. Low)

DOI: 10.3201/eid1409.080153

Table 1. Numbers of chlamydia tests, positive results, and change in positivity rates, Sweden, 2004–2006

Diagnostic test*	No. counties	No. positive results/total no. tests (%) in first 6 mo		
		2004	2005	2006
Abbott/Roche	14	11,721/150,080 (7.8)	11,111/147,311 (7.5)	10,236/152,960 (6.7)
Becton Dickinson	8	4,262/54,260 (7.9)	5,220/66,728 (7.8)	3,363/43,189 (7.8)
All tests	21	15,983/204,340 (7.8)	16,331/214,039 (7.6)	13,599/196,149 (6.9)

*One county used both Roche and Becton Dickinson tests.

quence targets (online Technical Appendix). The proportion of nvCT ranged from 20% to 64% in the 8 counties that used Abbott or Roche detection systems, compared with 7% to 19%, respectively, for counties that used BD tests (Figure 1). Additional data about gender, age, and clinical setting of diagnoses were available for 600 chlamydia-positive patients in the 4 counties using the BD system (Table 2). The proportion of nvCT cases varied between clinics ($p = 0.020$) and was higher at youth and venereal disease clinics than at antenatal and gynecology clinics. This variance might be because persons seeking treatment in these settings have higher levels of risk taking and more frequent changes in partners (4). There was no evidence of differences in the proportion of cases by gender ($p = 0.103$) or age ($p = 0.558$) because of nvCT.

Genetic characterization with a new high-resolution genotyping system (5) was performed on 48 specimens of nvCT from 2 counties that used the BD test system ($n = 21$); 2 counties that used Roche and Abbott systems ($n = 18$); and 9 specimens from Norway, Ireland, and France (online Technical Appendix). The nvCT showed a new genetic variant in the chromosomal target region *hctB* compared with previous findings in wild-type strains and thus constitutes a separate clone with the designation 21 (*hctB*), 19 (CT058), 1 (CT144), 2 (CT172), and 1 (*pbpB*) in our system. All 48 specimens tested were of genotype E, and 46 were identical in the *ompA* gene to the reference strain E/Bour. The divergent specimens were from 2 persons known to be sexual partners and differed in a single nucleotide position. In the other 5 target genes, altogether comprising some 5,500 bp, all 48 specimens were identical.

Conclusions

Our study was a national systematic overview including surveillance, demographic, microbiologic, and genetic data about the emergence and spread of a mutant strain of *C. trachomatis* in Sweden. A fall in the proportion of positive chlamydia test results in counties using Abbott or Roche test systems began in 2005 and continued in 2006, whereas positivity rates in counties using BD tests did not change. The mutant strain has now spread throughout Sweden. Notably, the new variant has scarcely been found outside Sweden (6), indicating that we need to improve our understanding of the sexual networks through which chlamydiae spread (7).

Our analysis suggests that widespread transmission of nvCT is recent, even if the mutation itself occurred some

time ago, because 46 of 48 specimens from different places had identical sequences when we used a highly discriminatory multilocus sequence typing system (5). This hypothesis is supported by the lack of diversification in the mutant strains compared with the high degree of sequence variation in other sample collections that we have analyzed (5; and unpub. data). We expect new nucleotide substitutions to occur over time.

The area in Sweden in which nvCT originated is not known, but the consistently high proportion of nvCT found in the county of Dalarna suggests that the mutant might have been present in this region for longer than in other counties studied. nvCT comprised 64% of chlamydia-positive specimens over the study period in Dalarna as a whole, and up to 78% in some localities (7); elsewhere in Sweden (8–10) and worldwide (11,12), genotype E strains of different subvariants comprise $\approx 40\%$ of chlamydia-positive specimens in heterosexual populations. These data might indicate that the high proportion of nvCT is not only a result of accumulation of chlamydia cases when diagnostics failed and treatment and contact tracing were inadequate. Further studies will be needed to determine whether nvCT also has a selective advantage that might outcompete the wild-type bacterium over time.

The emergence of this mutant strain of a sexually transmitted pathogen has implications for public health practice. A recent study estimates that some 8,000 chlamydia cases

Table 2. Distribution of cases of nvCT by gender, age, and clinic category in 4 selected counties that used the Becton Dickinson system*

Factor	% nvCT (n/N)	p value†
Gender		
Male	16 (45/273)	0.103
Female	12 (39/327)	
Age, y		
15–19	14 (23/162)	0.558
20–24	16 (44/279)	
25–29	11 (11/98)	
≥ 30	10 (6/59)	
Clinic		
Venereal disease	15 (19/129)	0.020
Youth clinics	19 (39/210)	
Gynecology	9 (13/150)	
Antenatal/general practice	8 (6/77)	
Others	21 (7/34)	

*nvCT, new variant of *Chlamydia trachomatis*; n, number of nvCT cases detected; N, total number of *C. trachomatis* cases detected.

†Determined by χ^2 test.

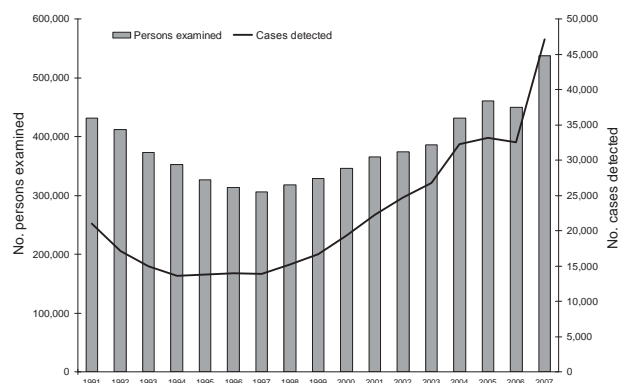


Figure 2. *Chlamydia trachomatis* reports, Sweden, 1991–2007. The number of persons examined and cases detected in 2007, when diagnostic tests for chlamydia had been changed, is in line with the increasing trend from 2004 and before. The figures for 2005 and 2006 reflect the failure to detect cases of the new chlamydia variant in some counties.

escaped detection in 2006 (7). This would have resulted in an $\approx 20\%$ increase in reported chlamydia cases. Actual national figures for 2007 confirm such an increase, and the number of reported chlamydia cases has reached an all-time high in Sweden (Figure 2). *Chlamydia* infections, caused not only by nvCT, continue to rise (13,14), but the areas most heavily affected by the spread of nvCT have been in much the same situation as before chlamydia was first recognized as a pathogen. Failure to detect the nvCT over time have resulted in episodes of complicated infection all over the country, leading to ectopic pregnancies and infertility. Research is now needed to determine whether sequelae associated with chlamydia occur disproportionately in counties where test systems fail to diagnose the nvCT. The ability of this new variant to escape detection for so long shows that developers of future diagnostic tests need to take into account the structure and function of genomes when selecting appropriate target nucleic acid sequences in microorganisms. Currently, there are unique opportunities for research that could lead to insights into the immunobiology, transmission, and consequences of *C. trachomatis*.

Acknowledgments

Prevalence data on the new variant of *C. trachomatis* or samples for analysis were provided from different counties. We thank Kenneth Persson, Ida Björklund, Torvald Ripa, Jens Björkman, Andreas Mattussek, Christina Lundberg, Hans Fredlund, Maria Rotzén Östlund, Britta Loré, and Barbro Almqvist. Amir Moghaddam generously contributed 6 specimens from Oslo, Norway, Yvonne Lynagh kindly provided 2 specimens from Ireland, and Bertille Barbeyrac provided 1 sample from France.

Research on the new variant of *C. trachomatis* was supported by grants from Roche Molecular Diagnostics and Becton Dickinson.

Dr Herrmann is a microbiologist and associate professor at the University Hospital in Uppsala, Sweden. His major research interests are diagnostics and epidemiology of *Chlamydia* infections and the development of molecular methods for detecting different bacteria and viruses.

References

1. Ripa T, Nilsson P. A variant of *Chlamydia trachomatis* with deletion in cryptic plasmid: implications for use of PCR diagnostic tests. *Euro Surveill.* 2006;11(11) [cited 2008 Apr 29]. Available from <http://www.eurosurveillance.org/ew/2006/061207.asp>
2. Ripa T, Nilsson PA. A *Chlamydia trachomatis* strain with a 377-bp deletion in the cryptic plasmid causing false-negative nucleic acid amplification tests. *Sex Transm Dis.* 2007;34:255–6.
3. Dellone B, Shank DD, Price JA. Analytical detection with the BD ProbeTec ET CT amplified DNA assay of a variant of *Chlamydia trachomatis* with a deletion in the cryptic plasmid. Presented at: 17th International Society for STD Research/10th International Union against Sexually Transmitted Infections Congress; 2007 Jul 29–Aug 1; Seattle, Washington, USA. Poster 144.
4. Herlitz C. HIV/AIDS and society: knowledge, attitudes and behaviour, 1987–2007 [in Swedish]. Article no. 2008:123–1. Stockholm: National Board of Health and Welfare; 2008.
5. Klint M, Fuxelius HH, Goldkuhl RR, Skarin H, Rutemark C, Andersson SG, et al. High-resolution genotyping of *Chlamydia trachomatis* strains by multilocus sequence analysis. *J Clin Microbiol.* 2007;45:1410–4. DOI: 10.1128/JCM.02301-06
6. Savage EJ, Ison CA, van de Laar MJ. Results of a Europe-wide investigation to assess the presence of a new variant of *Chlamydia trachomatis*. *Euro Surveill.* 2007 12(10) [cited 2008 Apr 29]. Available from <http://www.eurosurveillance.org/em/v12n10/1210-222.asp>
7. Herrmann B. A new genetic variant of *Chlamydia trachomatis*: a thrilling story in Sweden with global impact. *Sex Transm Infect.* 2007;83:253–4. DOI: 10.1136/sti.2007.026260
8. Jurstrand M, Falk L, Fredlund H, Lindberg M, Olcen P, Andersson S, et al. Characterization of *Chlamydia trachomatis omp1* genotypes among sexually transmitted disease patients in Sweden. *J Clin Microbiol.* 2001;39:3915–9. DOI: 10.1128/JCM.39.11.3915-3919.2001
9. Lysén M, Österlund A, Rubin CJ, Persson T, Persson I, Herrmann B. Characterization of *ompA* genotypes by sequence analysis of DNA from all detected cases of *Chlamydia trachomatis* infections during 1 year of contact tracing in a Swedish county. *J Clin Microbiol.* 2004;42:1641–7. DOI: 10.1128/JCM.42.4.1641-1647.2004
10. Persson K. Epidemiology of serovars of *Chlamydia trachomatis*. In: Bowie WR, Caldwell HD, Jones RB, Mardh PA, Ridgway GL, Schachter J, et al., editors. *Chlamydial infections*. Proceedings of the Seventh International Symposium on Human Chlamydial Infections. Cambridge (UK): Cambridge University Press; 1990. p. 559–62.
11. Geisler WM, Suchland RJ, Whittington WL, Stamm WE. The relationship of serovar to clinical manifestations of urogenital *Chlamydia trachomatis* infection. *Sex Transm Dis.* 2003;30:160–5. DOI: 10.1097/00007435-200302000-00013
12. van Duynhoven YT, Ossewaarde JM, Derksen-Nawrocki RP, van der Meijden WI, van de Laar MJ. *Chlamydia trachomatis* genotypes: correlation with clinical manifestations of infection and patients' characteristics. *Clin Infect Dis.* 1998;26:314–22. DOI: 10.1086/516291


13. Velicko I, Kuhlmann-Berenzon S, Blaxhult A. Reasons for the sharp increase of genital chlamydia infections reported in the first months of 2007 in Sweden. *Euro Surveill*. 2007;12(10) [cited 2008 Apr 29]. Available from: <http://www.eurosurveillance.org/em/v12n10/1210-223.asp>
14. Swedish Institute for Infectious Disease Control. Chlamydia infection, 2007 [cited 2008 Apr 8]. Available from <http://www.smittskyddsinstitutet.se/in-english/statistics/chlamydia-infection->

The opinions expressed by authors contributing to this journal do not necessarily reflect the opinions of the Centers for Disease Control and Prevention or the institutions with which the authors are affiliated.

Address for correspondence: Björn Herrmann, Department of Clinical Microbiology, Uppsala University Hospital, S-751 85 Uppsala, Sweden; email: bjorn.herrmann@medsci.uu.se

EMERGING INFECTIOUS DISEASES®

March 2008

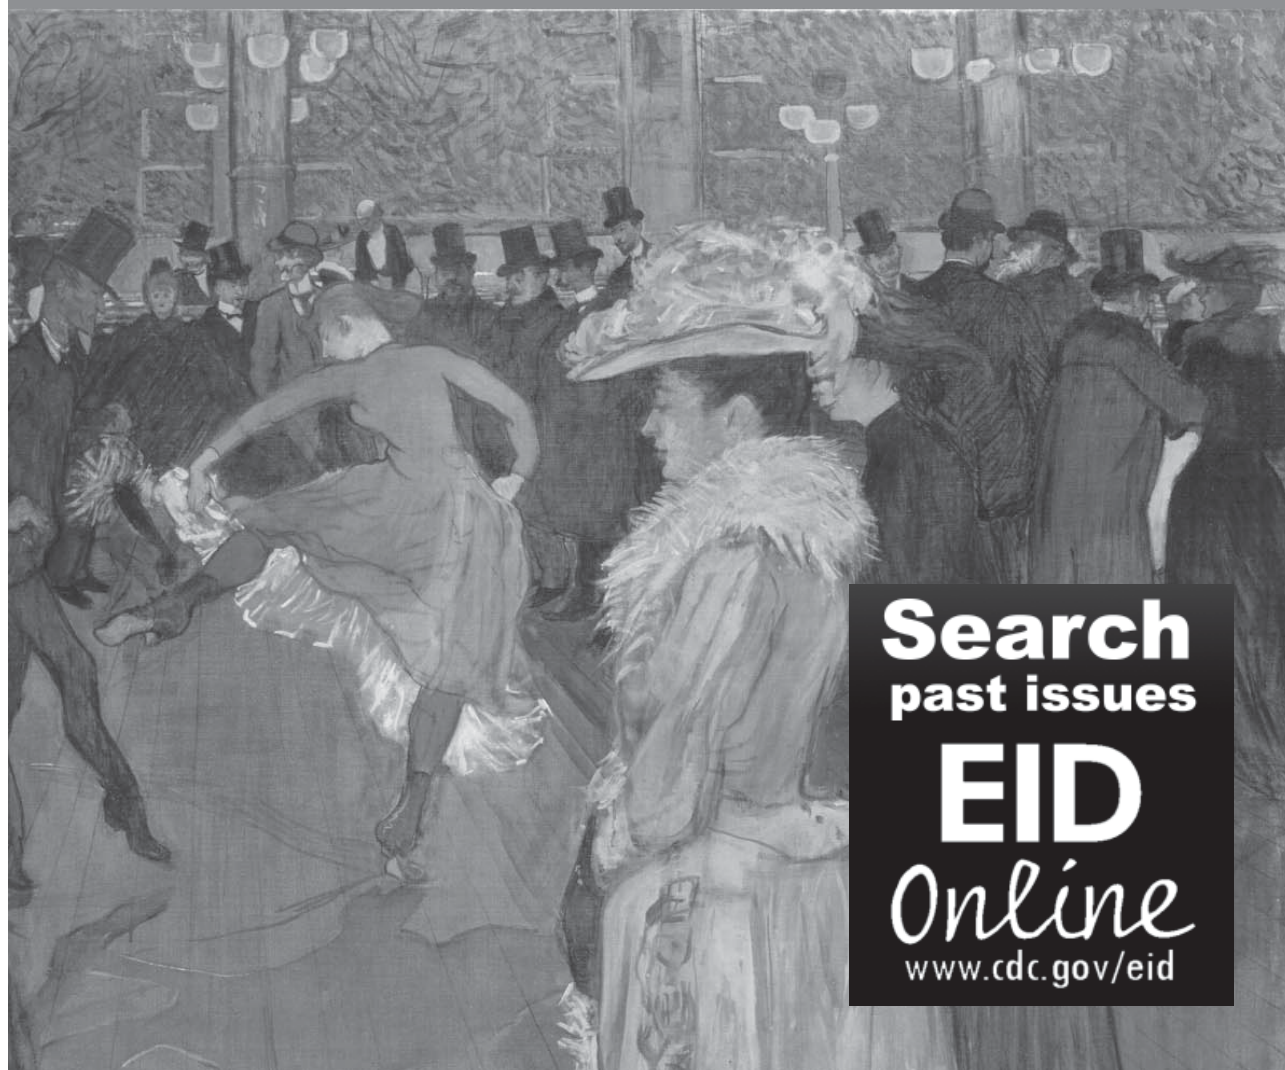

**Search
past issues**

EID
Online
www.cdc.gov/eid

Emergence and Spread of *Chlamydia trachomatis* Variant, Sweden

Technical Appendix

Analysis of National Surveillance Data

We used reports of diagnosed chlamydia infections reported to the Swedish Institute for Infectious Disease Control for the years 2004, 2005, and 2006. In late 2006, the institute recommended changes in laboratory diagnostic test systems to counties using Abbott (m2000) or Roche (COBAS Amplicor/TaqMan 48 CT ver 1) tests as a result of the new variant *Chlamydia trachomatis* (nvCT, see below). Because this could have affected patterns of testing and diagnosis, we restricted our analysis to data for the first 6 months of each year. First, we compared aggregated data from all counties from the first 6 months of 2004 and 2005, and calculated the relative change (with 95% confidence intervals [CI]) in the proportions of positive samples in counties using Abbott or Roche tests, and counties using the Becton Dickinson (BD) test. We then used a random effects model to examine the association between the diagnostic method and change in positivity rate between the first 6 months of 2005 and 2006. The model allowed for adjustment for the underlying time trend from 2005 to 2006, differences in positivity rates already present in 2005, and for county specific differences in coverage in testing of the target population. Examination of residual plots showed a good fit for the model.

Microbiologic Analysis

We collected data from consecutive samples tested over a period of 2 to 4 months in 12 counties between October 2006 and March 2007. From October 2006, all counties that used Abbott or Roche test systems for routine chlamydia diagnostics tested specimens in parallel with an assay using a target sequence not in the cryptic plasmid but in the chromosomal *ompA* gene (Artus *C. trachomatis* PCR, Qiagen, Hilden, Germany, or LightMix 480HT, TIB Molbiol, Berlin, Germany) (1), following a recommendation from the Swedish Institute for Infectious Disease Control. Discrepant cases were regarded as the new *C. trachomatis* variant.

Confirmation of nvCT was performed on subsets of discrepant cases by means of a real-time PCR specific to nvCT (2). In 4 counties (Norrbotten, Uppsala, Jönköping and Blekinge) that used the BD system for routine testing, consecutive chlamydia-positive specimens were collected from late November 2006 to February 2007. Urine samples were concentrated by centrifugation for 10 min at 5000 g and swab samples by Microcon centrifugation (Millipore) before DNA was purified using the MagAttract DNA mini kit (QIAGEN). The purified samples were reanalyzed with the Roche COBAS TaqMan 48 CT test. All specimens displaying discrepant results were tested by the PCR assay specific to nvCT (2). For each county we calculated the proportion of chlamydia positive specimens caused by nvCT. For the 4 counties that provided individual level data we compared the distribution of nvCT and wild type chlamydia cases according to gender, age, and diagnostic setting using chi-square tests.

Genetic Characterization

We used a new high-resolution genotyping system (3) to analyze specimens taken between October 2006 and March 2007. Specimens of nvCT were from 2 counties (Norrbotten, n = 7 and Uppsala, n = 14), which used the BD test system and from the counties Örebro, n = 13, and Skåne n = 5, which used the Roche and Abbott system, respectively. In addition, we analyzed 6 samples from Norway, 2 from Ireland and 1 from France. Accession numbers of sequences describing genetic variants found in the 48 nvCT specimens examined: CT058 type 19: EF690305; CT144 type 1: EF690306; CT172 type 2: EF690307; *hctB* type 21: EF690308; *pbpB* type 1: EF690309; *ompA*: EF690310 and X52557.

References

1. Unemo M, Olcén P, Agné-Stadling I, Feldt A, Jurstrand M, Herrmann B, et al. Experiences with the new genetic variant of *Chlamydia trachomatis* in Örebro county, Sweden—proportion, characteristics and effective diagnostic solution in an emergent situation. *Euro Surveill.* 2007;12:699.
2. Ripa T, Nilsson PA. A *Chlamydia trachomatis* strain with a 377-bp deletion in the cryptic plasmid causing false-negative nucleic acid amplification tests. *Sex Transm Dis.* 2007;34:255–6.
3. Klint M, Fuxelius HH, Goldkuhl RR, Skarin H, Rutemark C, Andersson SG, et al. High-Resolution Genotyping of *Chlamydia trachomatis* Strains by Multilocus Sequence Analysis. *J Clin Microbiol.* 2007;45:1410–4.