

NPPTL COVID-19 Response: International Respirator Assessment

Manufacturer: Guangdong Jiangmen Huayue Industrial Co. Ltd.

Model Tested: Three-Dimensional Protective Respirator (disposable respirator)

Date Tested: July 30, 2020

These findings pertain to the Guangdong Jiangmen Huayue Industrial Co. Ltd., Model Three-Dimensional Protective Respirator (disposable respirator). The packaging and labeling for this product indicates that it meets GB2626-2006 (the Chinese standard for Respiratory Protective Equipment – Non-Powered Air-Purifying Particle Respirator).

Ten respirators were submitted for evaluation. The samples were tested using a modified version of NIOSH Standard Test Procedure (STP) TEB-APR-STP-0059. This modified assessment plan can be found [here](#).

No certificate of approval was provided with the samples received; therefore, the authenticity of the claims cannot be validated.

The maximum and minimum filter efficiency was 85.10% and 31.50%, respectively. All respirators measured less than 95%.

While the above-listed product classification has similar performance requirements to NIOSH-approved devices, NIOSH does not have knowledge about the sustained manufacturer quality system and product quality control for these products. NIOSH also does not have knowledge about the product's handling and exposures after leaving its manufacturer's control.

In addition, this product is an ear loop design. Currently, there are no NIOSH-approved products with ear loops; NIOSH-approved N95s have head bands. Furthermore, limited assessment of ear loop designs, indicate difficulty achieving a proper fit. While filter efficiency shows how well the filter media performs, users must ensure a proper fit is achieved.

This assessment is not a part of the NIOSH respirator approval process and will in no way lead to or preclude NIOSH approval through the official approval process. This assessment was developed as an assessment of the filter efficiency for those respirators represented as certified by an international certification authority, other than NIOSH, to support the availability of respiratory protection to US healthcare workers due to the respirator shortage associated with COVID-19. Only particulate filter efficiency was assessed.

The results provided in this letter are specific to the subset of samples that were provided to NPPTL for evaluation.

These results will be used to update the CDC guidance for [Crisis Capacity Strategies \(during known shortages\)](#).

Evaluation of International Respirators

Test: Modified TEB-APR-STP-0059

Date Tested: July 30, 2020

Report Prepared: July 31, 2020

Manufacturer: Guangdong Jiangmen Huayue Industrial Co. Ltd.

Item Tested: Three-Dimensional Protective Respirator (disposable respirator)

Country of Certification: China (GB2626-2006)

Pictures have been added to the end of this report.

Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH ₂ O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency
1	85	6.9	66.3	66.4	33.60
2	85	7.5	63.2	34.2	65.80
3	85	9.9	14.9	14.9	85.10
4	85	7.5	66.6	66.7	33.30
5	85	6.5	63.1	63.1	36.90
6	85	5.7	60.3	61.0	39.00
7	85	7.0	68.1	68.5	31.50
8	85	10.3	18.2	18.2	81.80
9	85	5.8	59.6	59.6	40.40
10	85	5.4	63.6	63.9	36.10
Minimum Filter Efficiency: 31.50			Maximum Filter Efficiency: 85.10		


- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.



DR. HUAYUE
PURE AND HEALTHY

KN95 THREE-DIMENSIONAL
PROTECTIVE RESPIRATOR

Adopting KN95 grade anti-particulate matter filtering technology and antibacterial environmental protection fabric. Effectively filtering and protecting from PM2.5 air particulate matter and bacteria.

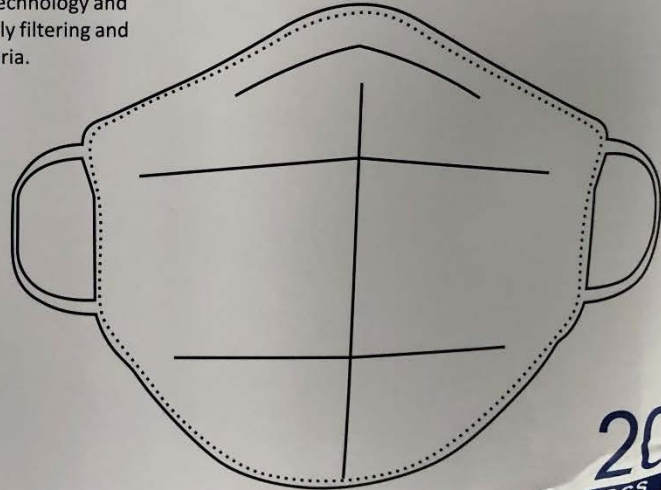

GB 2626-2006 KN95
(DISPOSABLE RESPIRATOR)

20
PCS




How To Wear:

1. Hold the respirator in hand, the fingertip is located in the nose clip, let the earband fall naturally.
2. Put the respirator over the face and make sure that the nose strip of the respirator is close to the nose to ensure tightness.
3. Pull the earband behind the ear.
4. Use two hands to adjust the whereabouts of the nose strips to ensure tightness.



Wearing Test:

- ◇ Use your hands to cover the mask and exhale, if you feel gas leaking from nose location, tighten the nose clip.
- ◇ If air leaks from the edge, readjust the earband to ensure tightness.

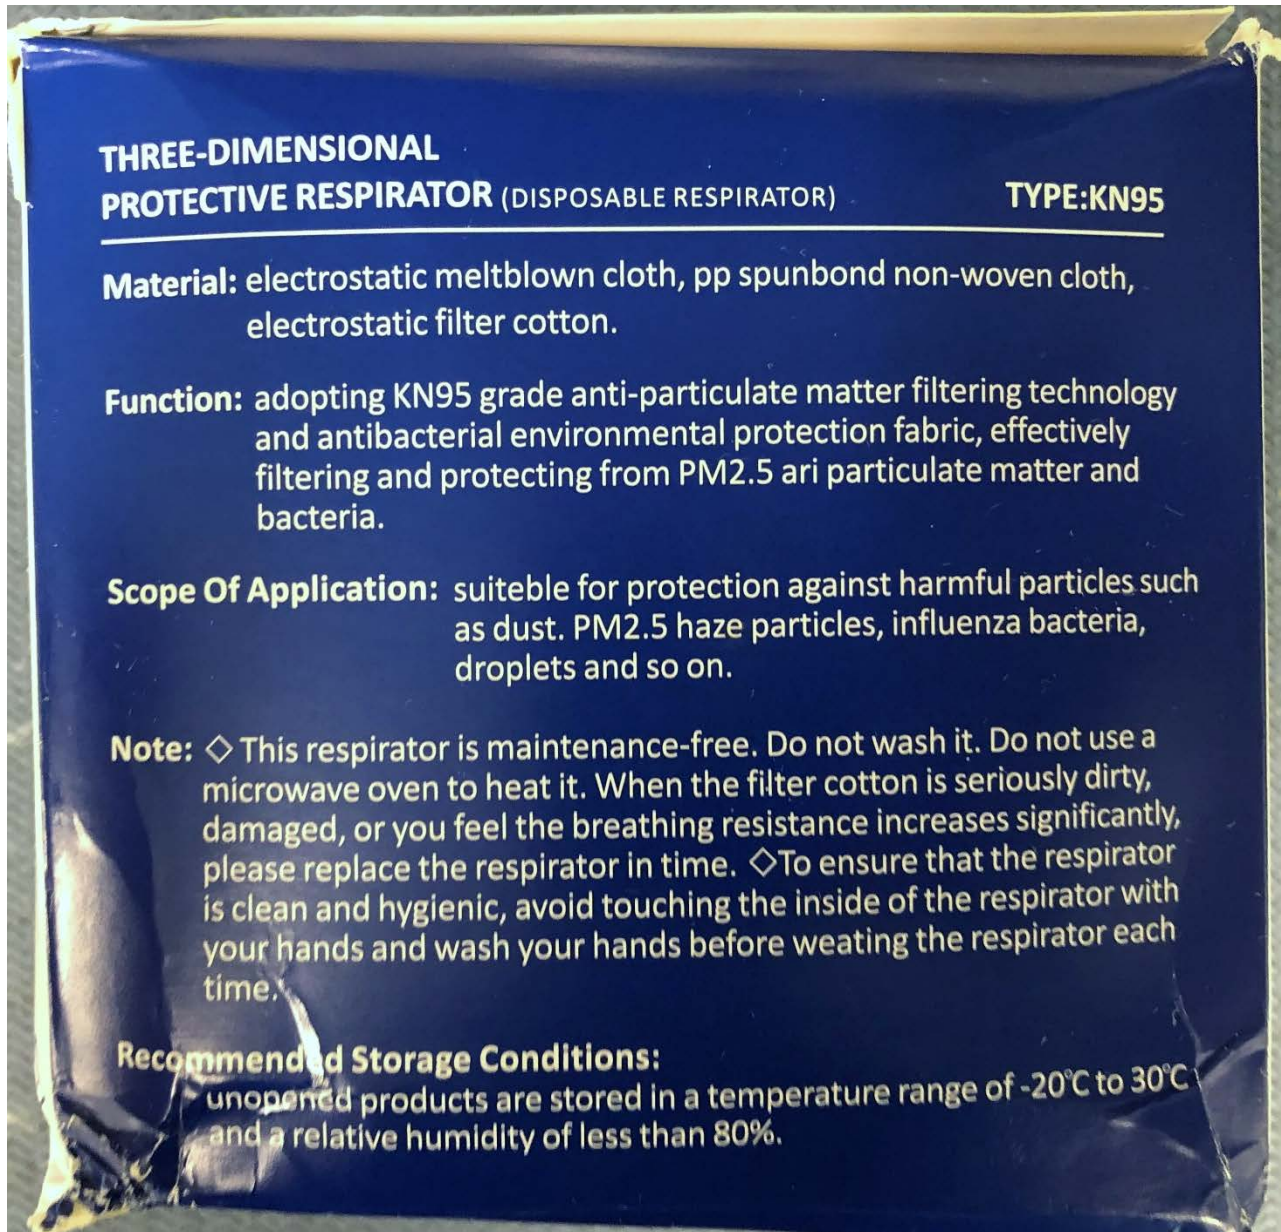

NPPTL COVID-19 Response: International Respirator Assessment

Note: the wearer must read and understand these instructions before using. Please save these instructions for reference.

Manufacturer: GUANGDONG JIANGMEN HUAYUE INDUSTRIAL CO.,LTD.
Address: Tangxia town, pengjiang district, jiangmen city, zhoujun village beach wai 14, no.1 factory Jiangmen, Guangdong, 529000, CHINA.
Implementation standard: GB 2626-2006 KN95
Production date: see packaging label
Shelf life 3 years (unopened)
Place of origin: Jiangmen, Guangdong
Phone:
Postcode: 529000



FFP2

MADE IN CHINA



**THREE-DIMENSIONAL
PROTECTIVE RESPIRATOR** (DISPOSABLE RESPIRATOR)

TYPE: KN95


Material: electrostatic meltblown cloth, pp spunbond non-woven cloth, electrostatic filter cotton.

Function: adopting KN95 grade anti-particulate matter filtering technology and antibacterial environmental protection fabric, effectively filtering and protecting from PM2.5 air particulate matter and bacteria.

Scope Of Application: suitable for protection against harmful particles such as dust, PM2.5 haze particles, influenza bacteria, droplets and so on.

How To Wear:

1. Hold the respirator in hand, the fingertip is located in the nose clip, let the earband fall naturally.
2. Put the respirator over the face and make sure that the nose strip of the respirator is close to the nose to ensure tightness.
3. Pull the earband behind the ear.
4. Use two hands to adjust the whereabouts of the nose strips to ensure tightness.

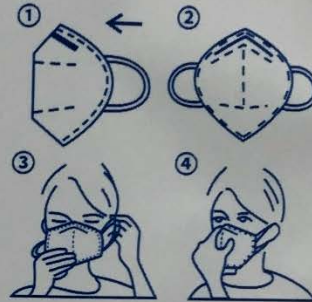

Wearing Test:

- ◇ Use your hands to cover the mask and exhale, if you feel gas leaking from nose location, tighten the nose clip.
- ◇ If air leaks from the edge, readjust the earband to ensure tightness.

Note:

- ◇ This respirator is maintenance-free. Do not wash it. Do not use a microwave oven to heat it. When the filter cotton is seriously dirty, damaged, or you feel the breathing resistance increases significantly, please replace the respirator in time.
- ◇ To ensure that the respirator is clean and hygienic, avoid touching the inside of the respirator with your hands and wash your hands before wearing the respirator each time.

Recommended Storage Conditions: unopened products are stored in a temperature range of -20°C to 30°C and a relative humidity of less than 80%.

Note: the wearer must read and understand these instructions before using. Please save these instructions for reference.

Manufacturer: GUANGDONG JIANGMEN HUAYUE INDUSTRIAL CO.,LTD.
Address: Tangxia town, pengjiang district, jiangmen city, zhoushan village beach wai 14, no.1 factory Jiangmen, Guangdong, 529000, CHINA.
Implementation standard: GB 2626-2006 KN95

Production date: see packaging label
Shelf life: 3 years(unopened)

Place of origin: Jiangmen, Guangdong

Phone:0750-3620188

Postcode: 529000



MADE IN CHINA



CE FFP2

QUALITY CERTIFICATE

Product name: three-dimensional protective respirator (disposable respirator)

Type: KN95

Materials: electrostatic melt blown cloth, pp spunbonded non-woven cloth, electrostatic filter cotton

Implementation standard:

GB 2626-2006 KN95

Hygienic standard:

GB 15979-2002

Production date: 2020-

Shelf life: three years (unopened)

Quality inspector: inspection 01

Guangdong Jiangmen Huayue Industrial Co.,Ltd.

NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment

