

anti-*Toxoplasma* Antibodies in Dried Blood Spots Proficiency Testing Program (TOXOPT)

Issued: February 28, 2018

Introduction

This report summarizes the data reported within the specified period for the Quarter 1, 2018, anti-*Toxoplasma* Antibody in dried blood spots (DBS) Proficiency Testing (PT) Program. It is distributed to all participants, state laboratory directors, and program colleagues by request. The tables within this report provide certification profiles for the distributed specimens, statistical analysis of the quantitative data, and frequency distribution summaries for expected interpretations. An evaluation of your laboratory's data is attached to this summary.

Certification of PT Specimens

This DBS panel was prepared from serum samples positive for *Toxoplasma* IgG and IgM purchased from SeraCare (Medford, Massachusetts) and from human serum positive for exposure to *Toxoplasma gondii* from a CDC specimen bank. All serum samples were mixed with washed red blood cells and the final hematocrit was adjusted to 50%. Table 1 provides the anti-*Toxoplasma* IgM expected values based on the NSQAP assayed values determined for each specimen by fluoroimmunoassay. Expected Clinical Assessments were based on a cutoff of 10 EIU/mL.

Table 1. NSQAP anti-*Toxoplasma* IgM Expected Values

Specimen	Expected Value (EIU/mL)	SD	Clinical Assessment
118T1	45.7	2.3	2
118T2	262.5	24.7	2
118T3	0.0	10.0	1
118T4	0.0	5.9	1
118T5	0.0	2.9	1

1 = *Toxoplasma* antibody non-reactive 2 = *Toxoplasma* antibody reactive

Distribution of PT Specimens

On January 9, 2018, a panel of five unknown DBS specimens was distributed to two laboratories in the United States and 13 laboratories in other countries.

Participant Results

◆ Quantitative Screening Results

We processed data from 11 participants. One laboratory submitted two sets of screening results. Laboratories were asked to report IgM screening results in Absorbance (OD) or other units. Five laboratories reported using an enzyme immunoassay method with units reported in OD, two reported using an enzyme immunoassay with units reported in EIU/mL, one used a fluorometric enzyme immunoassay (EIU/mL) to detect IgM, two reported using a Multiplex platform to report IgG (UA/mL), and one lab reported IgM and IgG results using a chemilumi-nescent immunoassay (CLIA). Overall statistics and cutoff information for the various immunoassay methods are summarized in Table 2. Extreme outlier data was removed from these statistics.

Table 2. Overall Statistics—Screening Results for Immunoassay Methods (N>1)

Method/ Antibody	Specimen	N	Mean	SD	Mean Reported Cutoffs	Range Reported Cutoffs
Enzyme Immunoassay IgM (OD) ^a	118T1	5	0.103	0.095	0.231	0.100—0.287
	118T2	5	0.410	0.256		
	118T3	5	0.031	0.017		
	118T4	5	0.030	0.018		
	118T5	5	0.031	0.024		
Enzyme Immunoassay IgM (EIU/mL) ^b	118T1	2	275.1	77.2	120.0	NA
	118T2	2	247.0	35.2		
	118T3	2	88.9	21.3		
	118T4	2	52.6	11.6		
	118T5	2	45.9	6.3		
Multiplex Immunoassay IgG (UA/mL) ^c	118T1	2	692.0	22.6	10.0	NA
	118T2	2	509.5	30.4		
	118T3	2	93.3	8.8		
	118T4	2	80.5	0.7		
	118T5	2	286.5	12.0		

^aOD = Absorbance Units

^bEIU/mL = Enzyme International Units/mL serum

^cUA/mL = Arbitrary Units/mL serum

◆ Quantitative Confirmatory Results

Participants were asked to confirm specimens that screened above their cutoff for sorting test results that were Toxoplasma-antibody reactive from those that were Toxoplasma-antibody non-reactive. Two laboratories provided confirmatory results using an enzyme immunoassay for IgG or IgM.

◆ Qualitative Clinical Assessments

Qualitative assessments may differ by participant because of specific assessment practices. Laboratory results were evaluated on the basis of the final assessments provided (screening only or confirmatory results). The frequency distribution of participant screening and confirmatory Clinical Assessments for both IgM and IgG are shown in Table 3.

Table 3. Frequency Distribution of Reported Clinical Assessments—All Methods

Type of Testing	Specimen	Toxoplasma antibody Non-reactive	Toxoplasma antibody Reactive
Screening	118T1*	4	8
	118T2	2	10
	118T3	12	0
	118T4	12	0
	118T5	10	2
Confirmatory	118T1*	1	1
	118T2	1	1
	118T3	2	0
	118T4	2	0
	118T5	2	0

*Specimen 118T1 was not evaluated due to lack of 80% consensus.

Evaluations

Overall, participants reported two False-negative and two False-positive final Clinical Assessments.

Future Shipments

The Newborn Screening Quality Assurance Program will ship next quarter's TOXOPT specimens on April 3, 2018

The content of this report may also be located on our website at:
http://www.cdc.gov/labstandards/nsgap_reports.html

**This program is co-sponsored by the Centers for Disease Control and Prevention (CDC) and
The Association of Public Health Laboratories (APHL)**


NEWBORN SCREENING QUALITY ASSURANCE PROGRAM

Direct inquiries to:

Centers for Disease Control and Prevention
4770 Buford Highway NE, MS/F19
Atlanta, GA 30341-3724
Phone: 404-488-7945 Email: jvm0@cdc.gov

Editors

Joanne Mei
Irene Williams

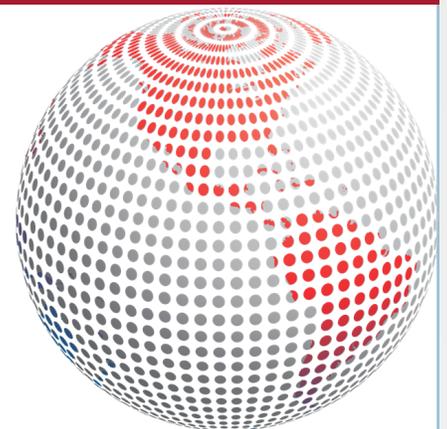

This *NEWBORN SCREENING QUALITY ASSURANCE PROGRAM* report is an internal publication distributed to program participants and selected program colleagues. The laboratory quality assurance program is a project cosponsored by the Centers for Disease Control and Prevention (CDC) and the Association of Public Health Laboratories.

CENTERS FOR DISEASE CONTROL AND PREVENTION (CDC) ATLANTA, GA 30341

Acting Director

Anne Schuchat, M.D. (RADM, USPHS)

Director

National Center for Environmental Health

Patrick Breysse, Ph.D.

Director

Division of Laboratory Sciences

James L. Pirkle, M.D., Ph.D.

Chief

Newborn Screening and Molecular Biology Branch

Carla Cuthbert, Ph.D.

Contributors:

Carter Asef

John Bernstein

Quan Bui

Preston Carter

Paul Dantonio

Sharon Flores

Elizabeth M. Hall

Christopher Haynes, Ph.D.

Brandon Kenwood

Francis Lee, Ph.D.

Lixia Li, Ph.D.

Timothy Lim, Ph.D.

Daniel Mandel, Ph.D.

Joanne Mei, Ph.D.

Kristina Mercer, Ph.D.

Gyliann Peña

Konstantinos Petritis, Ph.D.

Austin Pickens, Ph.D.

Robert Vogt, Ph.D.

Irene Williams

Sophia Winchester

Golriz Yazdanpanah

Sherri Zobel

Production:

Sarah Brown

Kimberly Coulter

Kizzy Stewart

ASSOCIATION OF PUBLIC HEALTH LABORATORIES SILVER SPRING, MD 20910

President

Ewa King, PhD

Chairman, Newborn Screening and Genetics in Public Health Committee

Michele Caggana, Sc.D., FACMG

Chairman, Newborn Screening Quality Assurance Quality Control Subcommittee

Patricia R. Hunt, B.A. and Joseph Orsini, Ph.D.

Chairman, Newborn Screening Molecular Subcommittee

Rachel Lee, Ph.D.

INQUIRIES TO:

Irene Williams, Editor • Centers for Disease Control and Prevention (CDC) • Newborn Screening Quality Assurance Program

Mailstop F-24 • 4770 Buford Highway, N.E. • Atlanta, GA 30341-3724

Phone (770) 488-4582 • NSQAPDMT@cdc.gov

E-mail: IWilliams1@cdc.gov