

Required Labeling of NIOSH Approved® N95® Filtering Facepiece Respirators

Approval Holder —

Name or logo of approval holder. If private labeled, the private label name or logo will appear instead of the approval holder information

NIOSH —

NIOSH name in block letters or NIOSH logo

TC-Approval Number (TC 84A-XXXX) —

For products manufactured after September 2008, the TC Approval Number is required to appear on the product

Model # XXXX —


Model Number or Part Number

Lot # XXXX —

Lot Number and Date of Manufacture (recommended, but not required)

Filter Designation* — NIOSH filter series. Alphanumeric rating followed by filter efficiency level (example, N95®, N99®, N100®, R95®, P95®, P100®) or Surgical N95 Respirator (when applicable)

*Registration symbol (®) will not appear on the actual product

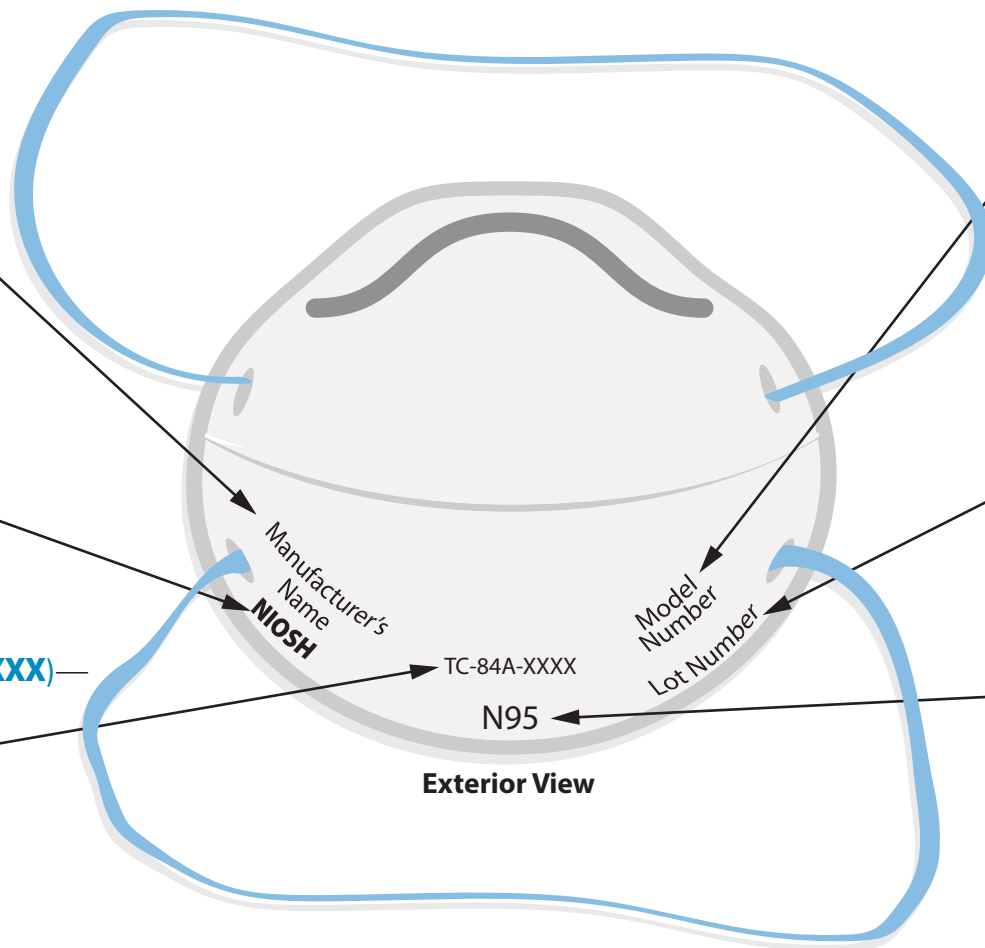

For more information, visit: www.cdc.gov/niosh/ppe/niosh-approved-respirators/index.html

N95 and NIOSH Approved are registered certification trademarks of the U.S. Department of Health and Human Services (HHS) in the United States and several other countries. The NIOSH stylized logo, N99, N100, R95, P95, and P100 are registered certification trademarks of the U.S. Department of Health and Human Services (HHS) in the United States.

Updated October 2026

