


Draft Guidance
 NIOSH CBRN Loose Fitting PAPR
 Certification Sequence and Quantity Requirements
 following the 42CFR Part 84 Requirements

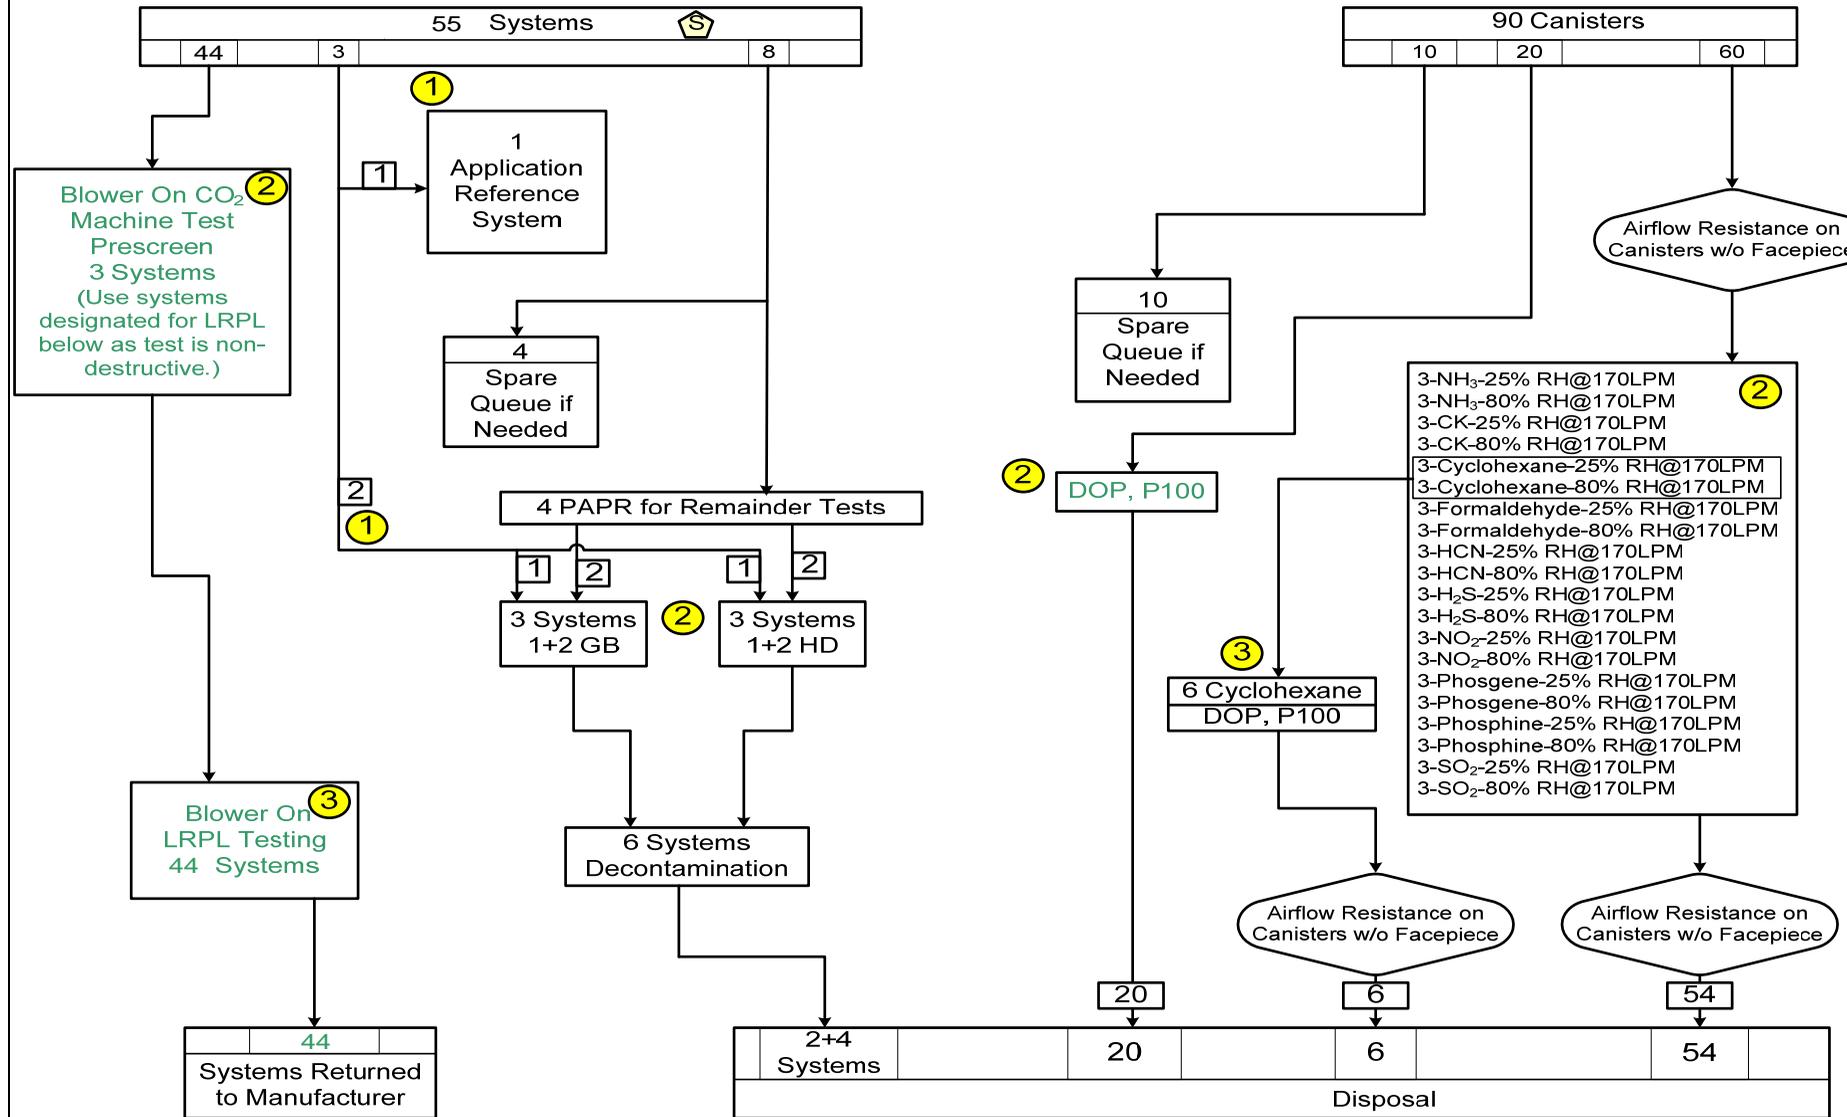

Model: Loose Fit
 Submitted by: PAPR Mfr.

Key

- Particulate Testing
- # Order of test to be completed before subsequent test begins.
- # Quantity of systems or canisters between tests
- S System is a Full Respirator Assembly in a Ready to Use configuration including canister and Minimum Packaging Configuration per User's Instructions.



National Institute for Occupational Safety and Health
NIOSH