


PPE CASE



Personal Protective Equipment Conformity Assessment Studies and Evaluations

Performance of Stockpiled Air-Purifying Respirators, Facility One of Ten: Inhalation and Exhalation Resistance and Filtration Efficiency Performance

National Institute for Occupational Safety and Health (NIOSH)

National Personal Protective Technology Laboratory (NPPTL)

Lee A. Greenawald, Susan M. Moore, Patrick L. Yorio, Kerri Wizner

March 1, 2020

In the event of a national emergency, eighteen million U.S. healthcare workers may face high-consequence infectious disease exposures [NIOSH 2017]. Personal protective equipment (PPE), such as gowns, gloves, goggles, and respirators, is an important measure within the infection prevention hierarchy of controls. During public health emergencies, the sudden increase in PPE demand may exceed supplies for upwards of three months while manufacturers increase production [ASTHO 2013; Carias et al. 2015]; [Patel et al. 2017]. For example, during the 2009 H1N1 pandemic, local respirator shortages were reported and, during the 2016 Ebola outbreak and the first U.S. fatality, there was a 10-200 fold increase in PPE orders [DHHS 2012; NIOSH 2018]. To prepare for these shortages, large quantities of PPE are strategically stockpiled at hospital, local, state, and federal facilities [NIOSH 1997].

Due to the decision to stockpile PPE, stockpile personnel and decision makers have sought to understand if stockpiled PPE is still viable following long-term storage. NIOSH does not require approval holders (i.e. those granted the approval from NIOSH) to designate a shelf life for particulate-only air-purifying respirators (APR), although some choose to do so and may provide this information on product packaging or online. There is limited published data to understand the viability of respirators that have undergone long-term storage with or without a designated shelf life. Over the past decade, the Strategic National Stockpile (SNS) and state and local stockpile personnel asked NIOSH to evaluate the performance of stockpiled PPE as well as better understand storage conditions in U.S. stockpile facilities that store PPE.

In 2017, NIOSH established a PPE Stockpile Partnership consisting of 1) federal entities and stockpiles; 2) state, county, and city stockpiles; 3) hospital-related stockpile entities; and 4) a manufacturer trade association to inform the design and execution of an empirical study to evaluate stockpiled APRs. NIOSH obtained samples of PPE from geographically dispersed stockpiles with varying storage conditions.

NIOSH found that 344 of 344 N95 filtering facepiece respirators stockpiled at Facility One that were 8-11 years old maintained their inhalation and exhalation resistance and filtration performance in accordance with NIOSH performance standards.

This report describes the inhalation/exhalation resistance and filtration performance of N95 filtering facepiece APRs collected from Facility One of Ten. This facility is a state stockpile facility.

How NIOSH Evaluated Respirators and Storage Conditions

Description of Facility One

- NIOSH researchers visited Facility One in August 2017 (**Figure 1**). This facility was located within the U.S. Department of Health and Human Services Region 2, representing New York, New Jersey, Puerto Rico, and the Virgin Islands.

Assessment of Storage Conditions

- NIOSH, in conjunction with the PPE Partnership members, developed checklists to document site and packaging (i.e. pallet, case, and box) conditions that may impact respirator performance.
- NIOSH documented the following storage conditions: 1) the PPE packaging presence of dust, shrink-wrapping, chemicals, and moisture, 2) exposure to sunlight and direct light; 3) proximity to fans, windows, doors, and ventilation systems; 4) damage to pallet and product packaging; and 5) location of pallet on storage rack (e.g., top, bottom) and location of PPE product on pallet (e.g., top/not load-bearing, bottom/load-bearing).



Figure 1: NIOSH documented storage practices at Facility One such as location and type of lighting, pallet stacking practices, and conditions of the flooring, roofing, and exterior walls.

- NIOSH reviewed facility temperature and percent relative humidity (%RH) data provided by Facility One stockpile personnel. This data was collected in 30-minute intervals from March 2014 to February 2017.

Collection of Respirator Samples

- Facility One's inventory included APRs that are classified as N95 filtering facepiece respirators (FFRs). Samples were collected from three different manufacturing models¹: 1) 3M 1860 (two different manufacturing years); 2) Gerson 1730; and 3) Medline/Alpha ProTech (APT) NON27501² (**Table 1**).
- Upon reviewing the detailed APR inventories and storage location by lot within Facility One, two different manufacturing lots for each model were identified and sampled within Facility One. Two lots

¹ Based on the other nine collaborating stockpiles' inventories, these three models were sampled in order to compare performance within common respirator models when stored under disparate conditions.

² The FFR model NON27501 has been manufactured by Alpha ProTech as a private label to Medline under TC-84A-0457.

- were sampled to evaluate and attempt to account for inter-lot variation. Products were collected and shipped to the NIOSH facility overnight to reduce exposure to non-climate-controlled conditions.
- Forty-three respirators were tested from each manufacturing lot for inhalation and exhalation resistance (n=3) and filtration performance testing (n=40)³.

Selection of Control Respirators

- Control respirators of the same model as those sampled from the facility were purchased from the open market to be used as a comparison between stockpiled and new respirators.

Characteristics of Sampled Respirators

- Table 1** provides a summary of the respirator models sampled from Facility One.

Table 1. FFRs Sampled from Stockpile Facility One

Model	Lot #	Year of Manufacture	Shelf Life on Packaging?	Respirator Age at Time of Testing ⁴	Shelf Life Status at Time of Testing
3M 1860	Lot A	2009	No	8 years	Past 5-year shelf life ⁵
3M 1860	Lot B	2009	No		
3M 1860	Lot A	2008	No	9 years	Past 5-year shelf life ³
3M 1860	Lot B	2008	No		
Gerson 1730	Lot A	2006	No	11 years	No shelf life designated
Gerson 1730	Lot B	2006	No		
Medline/APT NON 27501	Lot A	2008	No	9 years	No shelf life designated
Medline/APT NON27501	Lot B	2008	No		

Evaluation of Inhalation and Exhalation Resistance and Filtration Performance

- Twenty-three control respirators were tested for inhalation and exhalation resistance and filtration performance. The Gerson 1730 and Medline/APT NON27501 controls were manufactured in 2017 and the 3M 1860 controls were manufactured in 2018. NIOSH testing requirements state that a minimum of three respirator units must be tested for inhalation and exhalation resistance. The same three respirators can be used for both inhalation and exhalation resistance testing [NIOSH 2018].
- Inhalation and exhalation resistance and filtration performance of the stockpiled and control respirators were evaluated using the same Standard Test Procedures (STPs) NIOSH uses for approving respirators under 42 Code of Federal Regulations Part 84, “Approval of Respiratory Protective Devices” [NIOSH 2018] (**Table 2**).
- Table 2** describes the method for evaluating the inhalation and exhalation resistance and filtration performance of sampled respirators and control respirators.

³ NIOSH testing requirements state that a minimum of three respirator units must be tested for inhalation and exhalation resistance and a minimum of 20 must be tested for filtration efficiency [NIOSH 2018].

⁴ Testing was completed in 2017.

⁵ In 2013, 3M designated a five-year shelf life for the 3M 1860 model [3M 2018]. As of February 2020, this model still has a five-year shelf life.

Table 2. NIOSH Tests Conducted to Evaluate Inhalation and Exhalation Resistance and Filtration Performance.

NIOSH Standard Test Procedures (STPs)	Pass/Fail Criteria for APRs	Stockpiled Respirators Tested Per Manufacturing Lot	Control Respirators Tested
STP 3: Exhalation Resistance	<25 mm H ₂ O column @ 85 liters per minute (LPM)	3 ⁶	3 ⁶
STP 7: Inhalation Resistance	<35 mm H ₂ O column @ 85 LPM	3 ⁶	3 ⁶
STP 59: Particulate Filter Efficiency for N95	≤5.0% particulate penetration ($\geq 95.0\%$ filter efficiency)	40 ⁷	20

What NIOSH Found Through Inspection, Testing, and Evaluation

Storage Conditions

- Visual Inspections—Dust and damage to product packaging was limited or not observed at Facility One; examples of the most amount of dust and damage to product packaging are shown in **Figures 2 and 3**. Of the 344 respirators visually inspected, only one concern was noted, which was a slight deformation to one Gerson 1730 respirator (**Figure 4**).



Figure 2: Most amount of dust observed on product cases from Facility One.

⁶ NIOSH testing requirements state that a minimum of three respirator units must be tested for inhalation and exhalation resistance. The same three respirators can be used for both inhalation and exhalation resistance testing.

⁷ An increased sample size was used for the stockpiled respirators as opposed to the control respirators to increase the precision of the performance estimates investigated.



Figure 3: Most amount of product case damage observed from Facility One.

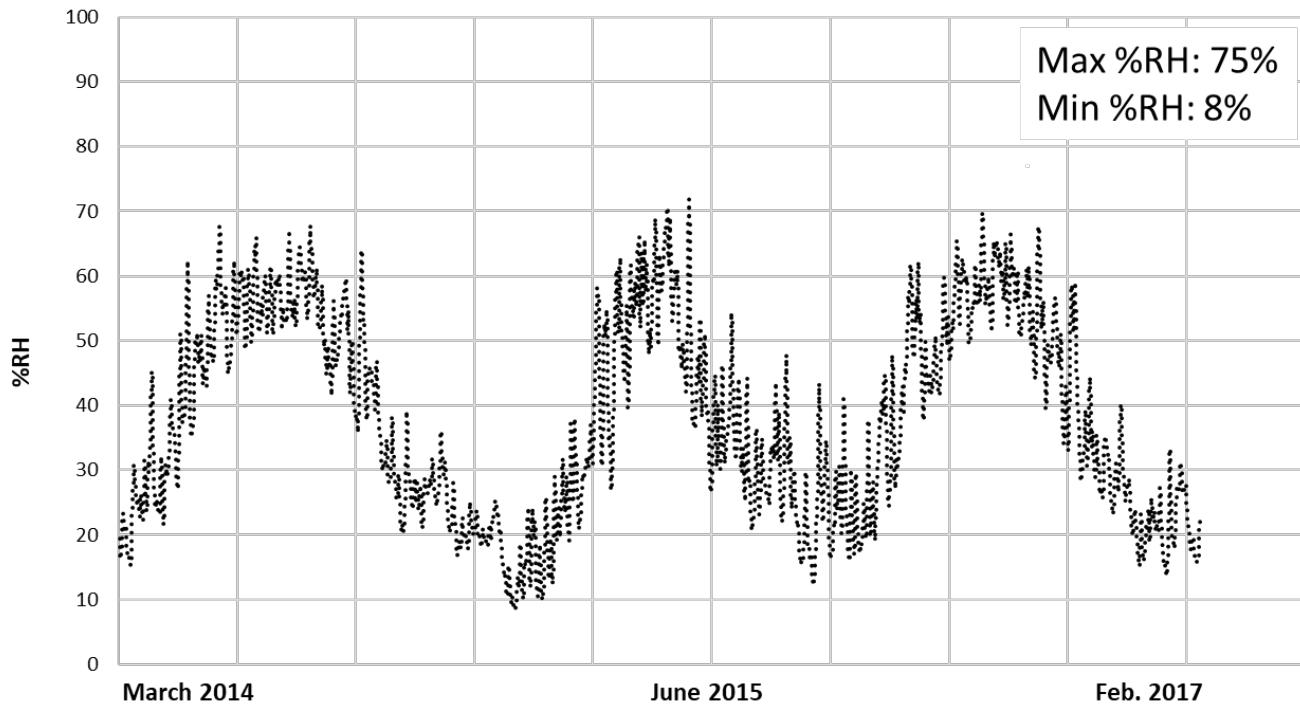


Figure 4: Most amount of product damage observed from Facility One.

- Temperature was controlled; temperature and %RH were monitored. Facility lights were off when not in use and no windows allowed sunlight to enter the facility. No evidence of excess moisture or chemical spills that persisted beyond immediate mitigation were observed. Pallets were shrink wrapped around the four pallet sides but not across the top or bottom. With the exception of the top-most row, pallets were separated by racks. On the top-most row, pallets were stacked two-high causing some weight/load to be applied to the bottom pallet.
- Percent RH (**Figure 5**) and Temperature (**Figure 6**)
 - At the time of publication, the recommended storage requirements for %RH and temperature are
 - 3M 1860: remain under 80 %RH; remain within -4°F to 86°F [3M 2017]
 - Gerson 1730: remain under 80 %RH; remain within -4°F to 95°F [Gerson 2019]
 - Medline/APT NON27501: avoid excessive moisture (water droplets or direct submersion in water); avoid prolonged extreme temperatures (< 60°F and >80°F) [Alpha ProTech 2019]
 - The average temperature between the 2014-2017 time period was 71.3°F. The average %RH between 2014-2019 was 38.3%; these averages are within the 3M, Gerson, and APT recommended temperature and %RH storage conditions.
 - No %RH or temperature data points deviated from the recommended storage conditions for the 3M 1860, Medline/APT, or the Gerson 1730 respirator models.

-
- Some respirators from Facility One were previously stored and deployed from a federal SNS facility. Although the current tracking process does not allow for retrieval of the historical location(s) and environmental conditions for these sampled products, subsequent discussions with SNS leadership suggest that SNS storage conditions met the recommended conditions.

Data Logger 1



Data Logger 2

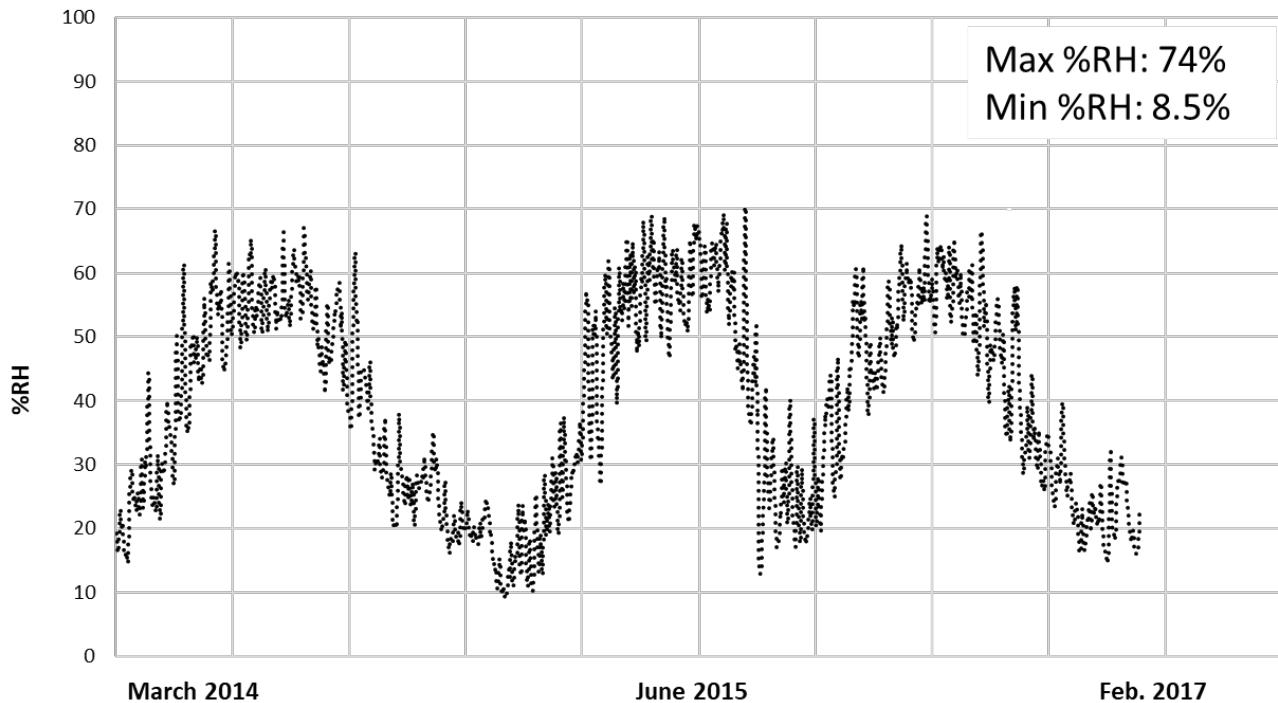


Figure 5: Percent Relative Humidity (% RH) from March 2014 – February 2017 for two data loggers stored at Facility One. Data is plotted as a 50-point moving average for visualization purposes. Maximum and minimum temperatures reported are noted for each data logger.

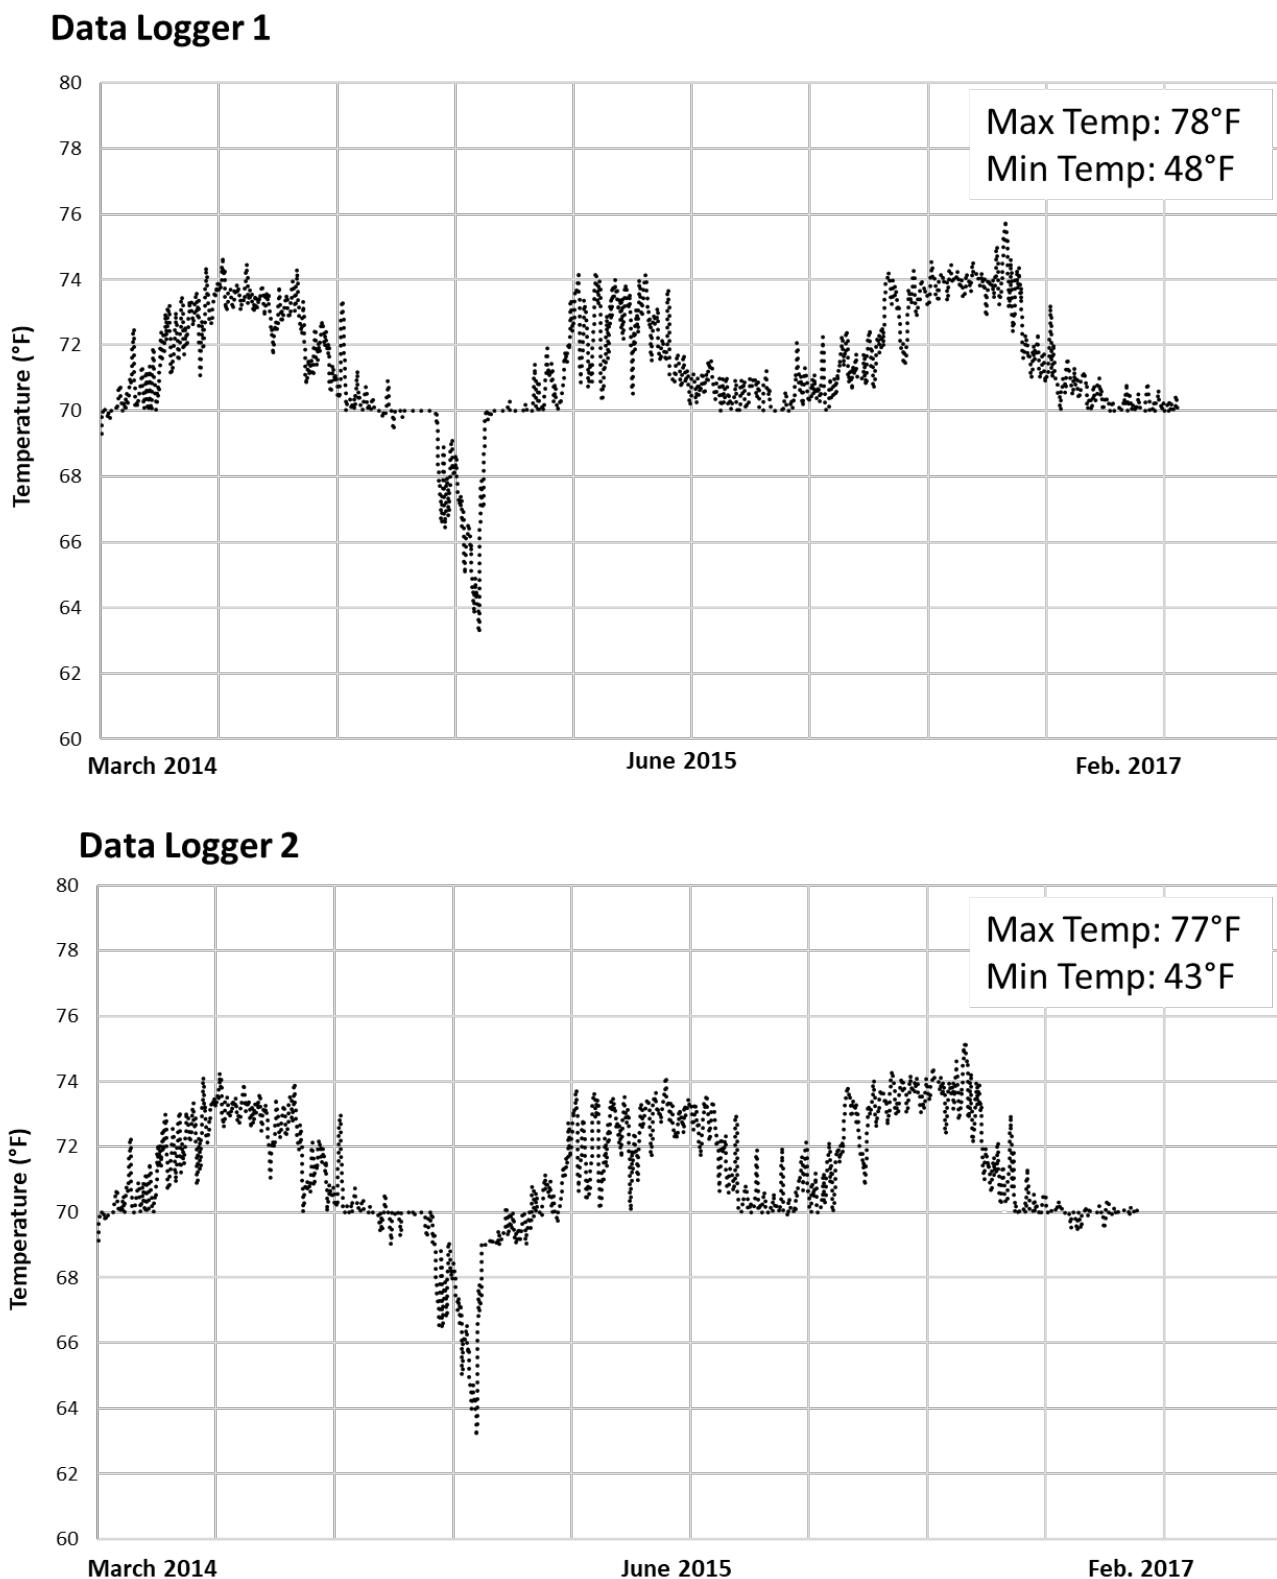


Figure 6: Temperatures from March 2014 – February 2017 for two data loggers stored at Facility One. Data is plotted as a 50-point moving average for visualization purposes. Maximum and minimum temperatures reported are noted for each data logger.

Inhalation and Exhalation Resistance

- NIOSH evaluated the inhalation and exhalation resistance for a total of 24 stockpiled and 9 control respirators. **All stockpiled and control respirators from each model passed these tests (Figure 7).**
- Using an analysis of variance (ANOVA), there were no statistically significant differences (defined as $\alpha \leq 0.05$) between the FFR controls and FFR stockpiled respirators for inhalation and exhalation resistance when averaging across models.
- When comparing the individual respirator models to their respective controls through an ANOVA with adjusted, post-hoc multiple comparisons, the following statistically significant differences were detected: 1) Gerson 1730 stockpiled Lot A had a statistically higher inhalation resistance; 2) Gerson 1730 stockpiled Lot A had a statistically higher exhalation resistance; and 3) Medline/APT NON27501 stockpiled Lot B had a statistically lower exhalation resistance. The mean inhalation and exhalation resistances values are shown in **Figure 7**.
- For inhalation resistance, the individual stockpiled respirator with the highest resistance (11.93 mm H₂O) was below the NIOSH maximum limit for product approval (35 mm H₂O allowable maximum). For exhalation resistance, the individual stockpiled respirator with the highest resistance (11.43 mm H₂O) was below the NIOSH maximum limit for product approval (25 mm H₂O allowable maximum).

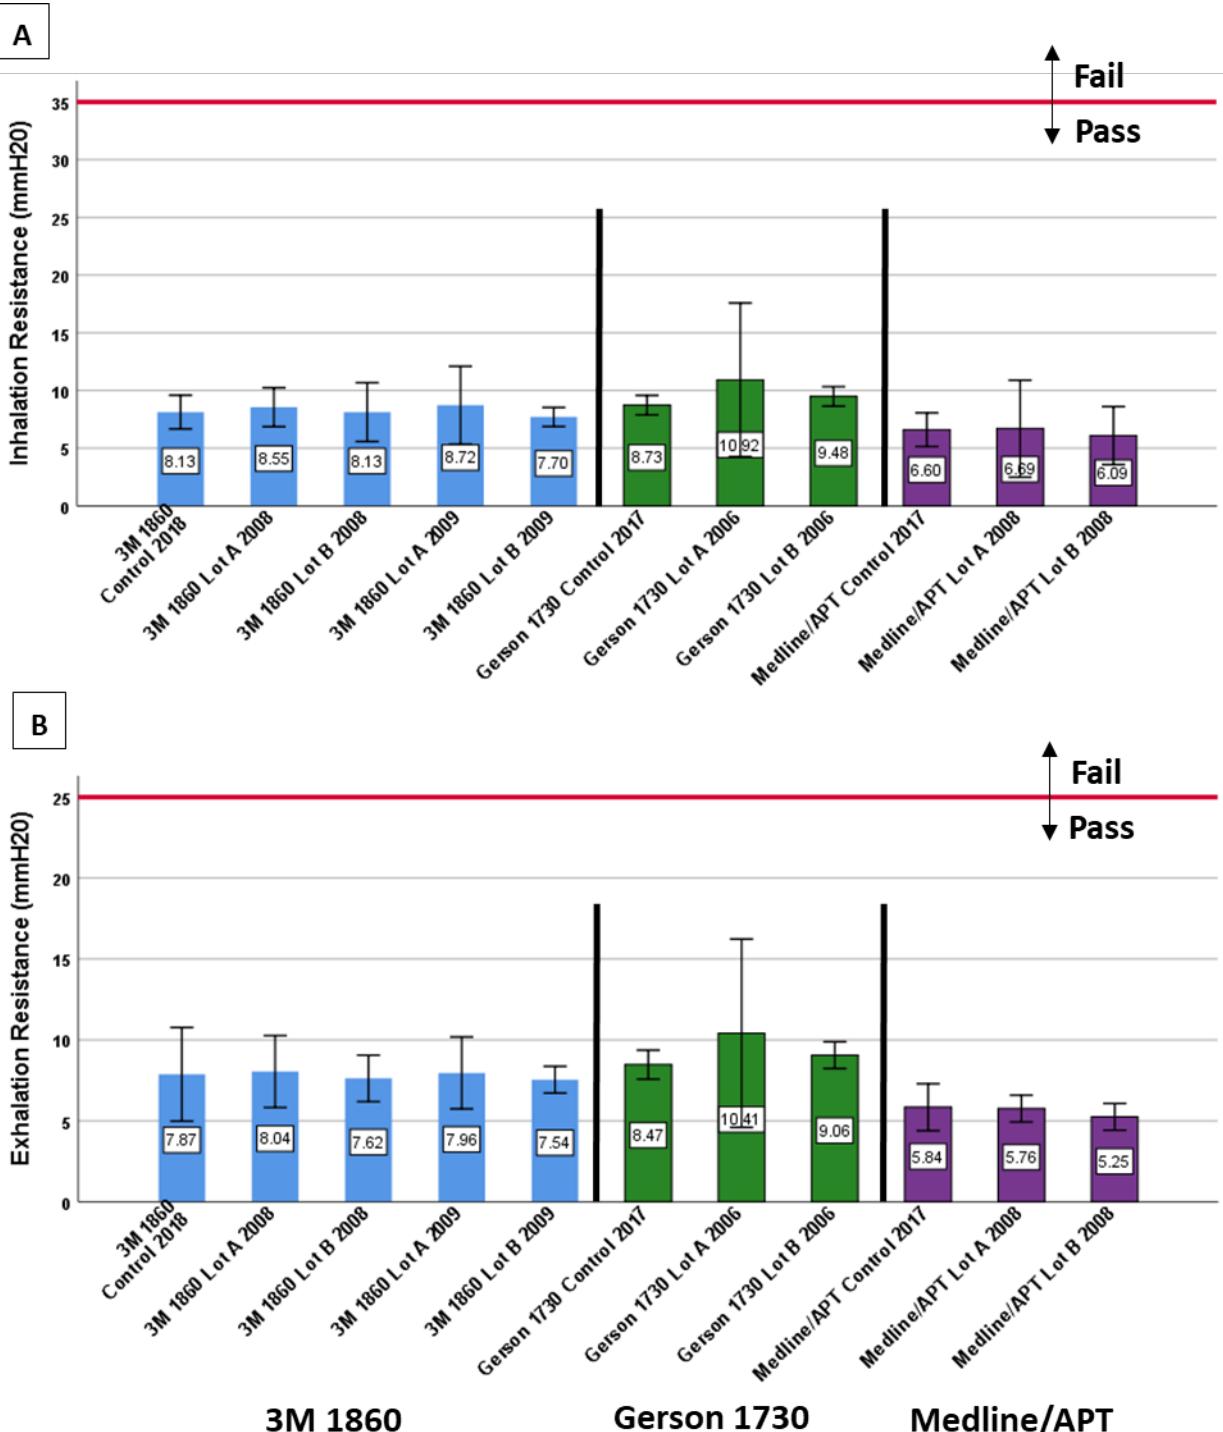


Figure 7: Control and stockpiled respirator inhalation (A) and exhalation (B) resistance data. N95 FFRs must have an inhalation resistance less than 35 mmH₂O and an exhalation resistance less than 25 mmH₂O. The pass/fail threshold for inhalation (A) and exhalation (B) resistance is shown by the red line. Error bars represent the 99% confidence interval and estimate the population parameters. This confidence interval suggests that 99% of any repeated samples tested and evaluated from this lot will have a mean between the upper and lower bounds.

Filtration Performance

- NIOSH evaluated the particulate penetration efficiency for 320 stockpiled respirators and 60 controls. **All stockpiled and control respirators from each model passed this test (Figure 8).**
- Using an analysis of variance (ANOVA), there were no statistically significant differences (defined as $\alpha \leq 0.05$) between the FFR controls and FFR stockpiled respirators for filtration when averaging across models.
- When comparing the individual respirator models to their respective controls through an ANOVA with adjusted, post-hoc multiple comparisons, the following statistically significant differences were detected: 1) 3M 1860 stockpiled 2008 Lot A had a higher penetration; 2) 3M 1860 stockpiled 2009 Lot B had a higher penetration; 3) Gerson 1730 stockpiled Lot B had a higher penetration; and 4) Medline/APT NON27501 stockpiled Lot A and B had a statistically significantly lower penetration. The mean percent particle penetration for each lot of respirators tested is shown in **Figure 8**.
- The individual stockpiled respirator with the highest penetration (4.43%) was nearly identical to the control respirator with the highest penetration (4.44%), with both being below the NIOSH maximum limit for product approval (5.0% penetration allowable).
- Additionally, the respirator shown in **Figure 4** that had a visual inspection concern had a value of 1.00% maximum penetration when tested and, therefore, was not the stockpiled respirator associated with the highest penetration.

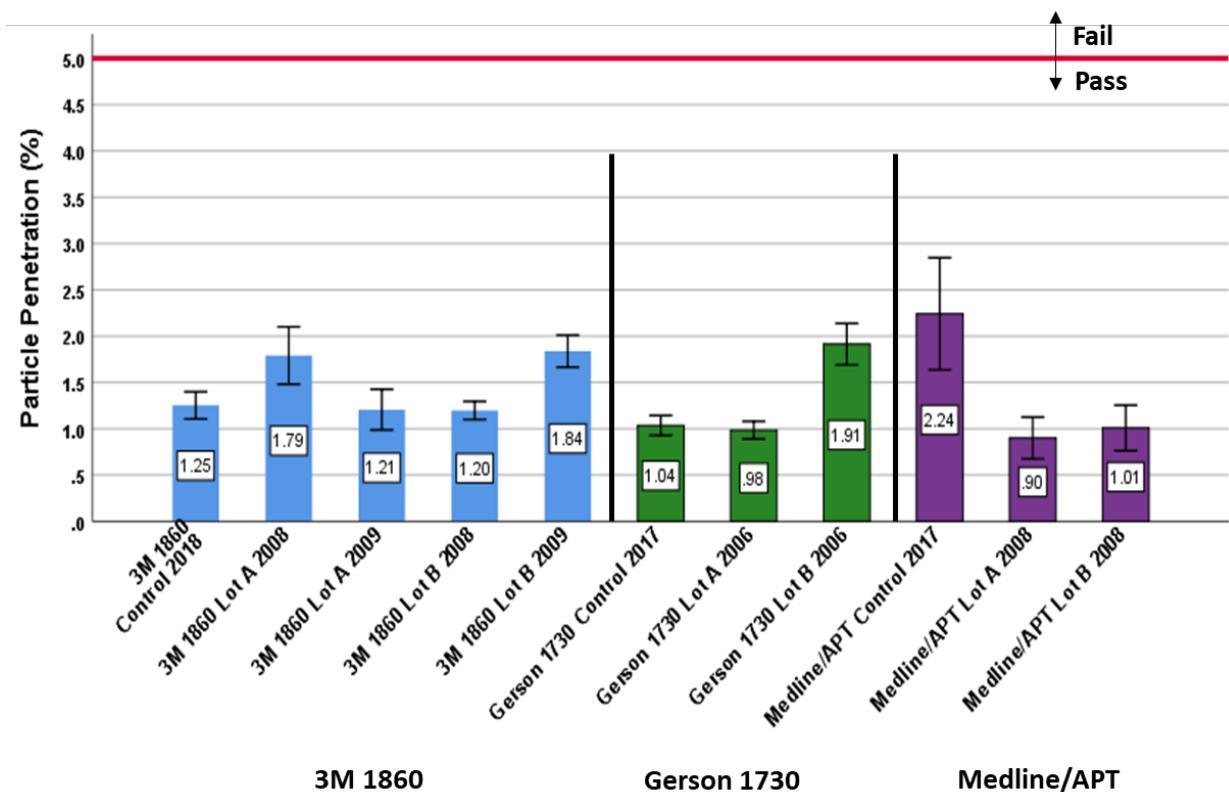


Figure 8: Control and stockpiled respirator particle filtration performance data. N95 FFRs must have a particle penetration of less than 5.0%. Error bars represent the 99% confidence interval and estimate the population parameters. This confidence interval suggests that 99% of any repeated samples tested and evaluated from this lot will have a mean between the upper and lower bounds.

CASE Findings

Findings for the Gerson 1730 Model:

No failures for inhalation resistance, exhalation resistance, or filtration performance were observed—i.e., the performance data suggests that these units would be protective so long as a proper fit is achieved. No shelf life was designated for this model by the approval holder. These findings pertain to Gerson 1730 units from Facility One and may not be applicable to other stockpile facilities and/or under different environmental storage conditions.

Findings for the 3M 1860 Model:

No failures for inhalation resistance, exhalation resistance, or filtration performance were observed—i.e., the performance data suggests that these units would be protective so long as a proper fit is achieved. This model currently has a five-year shelf life; Appendix 1 shows a 3M letter to end users with shelf life and recommended storage condition information [3M 2020]. Thus, these respirators tested are past their designated shelf life. These findings pertain to 3M units from Facility One and may not be applicable to other stockpile facilities and/or under different environmental storage conditions.

Findings for the Medline/Alpha ProTech NON27501 Model:

No failures for inhalation resistance, exhalation resistance, or filtration performance were observed—i.e., the performance data suggests that these units would be protective so long as a proper fit is achieved. No shelf life was designated for this model (Appendix 2, [Alpha ProTech, 2020]). These findings pertain to Medline/Alpha ProTech units from Facility One and may not be applicable to other stockpile facilities and/or under different environmental storage conditions.

Stockpile Storage Conditions:

The data made available by Facility One to the NIOSH research team suggests that all three respirator models evaluated in this study were stored in an environment that was within the previously described recommendations for %RH and temperature. Stored under these conditions, NIOSH found that the 344 N95 FFRs evaluated in this study, which were 8-11 years old, maintained their inhalation and exhalation resistance and filtration performance (i.e., all respirators were below the NIOSH maximum limit as defined by 42 CFR Part 84).

NIOSH regulation sets the minimum quality and performance requirements for the approval of respirators [NIOSH 1997]. NIOSH does not have requirements for shelf life or storage conditions for particulate-only APRs. The approval holder⁸ (i.e. the entity that is granted the approval from NIOSH) is responsible for understanding how their products' design or performance may be affected by various use or storage conditions and must provide instruction for establishing the proper use, storage, and maintenance procedures for their approved products, which may include designating a shelf life [NIOSH 2019]. FFR or particulate filter packaging (such as the box) often includes NIOSH-approved user instructions, label information, and recommendations on shelf life. Additionally, some approval holders also disseminate recommendations related to storage and shelf life through

⁸ An approval may be granted to a non-manufacturing entity.

resources such as user and web notices. The respirators tested in this study were generally not designed for long-term storage.

At this time, we do not have enough information to definitively know the level of protection that may be provided by respirators that 1) are stored for prolonged periods of times; 2) are stored under various storage conditions; or 3) have exceeded the approval holder's designated shelf life. Users of respirators that have exceeded the designated shelf life should be forewarned to avoid a false sense of confidence; these devices may not provide the same level of protection as those that have not exceeded the designated shelf life. We recommend contacting the approval holder(s) of the respirators in the stockpile with specific questions regarding the use of product beyond the designated shelf life.

What Can Stockpile Personnel Do to Learn More about the Respirators in their Stockpile?

- Stockpile personnel should check the product information from the approval holder as well as the NIOSH Certified Equipment List to remain up-to-date on product storage conditions, shelf-life information, and NIOSH approval status. Check NIOSH's Certified Equipment List to verify the respirator model currently maintains its NIOSH approval at
<https://www.cdc.gov/niosh/npptl/topics/respirators/cel/default.html>
- Stockpile personnel should work with the approval holder(s) of the stockpiled products with specific questions regarding the use of expired product.
- Sign up for NPPTL's Listserv at <https://www.cdc.gov/niosh/npptl/sub-NPPTL.html> to receive email notifications relevant to PPE.

For more information related to personal protective equipment, visit the [NIOSH NPPTL website](#)
<https://www.cdc.gov/niosh/npptl/>

Get More Information

Find NIOSH products and get answers to workplace safety and health questions:

1-800-CDC-INFO (1-800-232-4636) | TTY: 1-888-232-6348

CDC/NIOSH INFO: cdc.gov/info | cdc.gov/niosh

Monthly NIOSH eNews: cdc.gov/niosh/eNews

All photos courtesy of NIOSH NPPTL.

Disclaimer

The recommendations in this report are made based on the findings at the stockpile evaluated and may not be applicable to other stockpile facilities.

Mention of any company or product does not constitute endorsement by the National Institute for Occupational Safety and Health (NIOSH). In addition, citations to websites external to NIOSH do not constitute NIOSH endorsement of the sponsoring organizations or their programs or products. Furthermore, NIOSH is not responsible for the content of these websites. All web addresses referenced in this document were accessible as of the publication date.



Centers for Disease Control
and Prevention
National Institute for Occupational
Safety and Health

Suggested Citation

NIOSH [2020]. PPE CASE: Inhalation and Exhalation Resistance and Filtration Performance of Stockpiled Air-Purifying Respirators: Facility One of Ten. By Greenawald, L., Moore, S., Yorio, P., and Wizner, K. Pittsburgh, PA U.S. Department of Health and Human Services, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, NPPTL Report Number P2020-0101.

References

3M [2017]. Frequently Asked Questions: 3M Filtering Facepiece/Disposable Respirator Storage Conditions and Shelf Life. St. Paul, MN. <https://multimedia.3m.com/mws/media/10158530/faq-3m-filtering-facepiece-disposable-respirator-storage-conditions-and-shelf-life.pdf> [accessed February 27, 2020].

3M [2018]. 3M Personal Safety Division Letter. St. Paul, MN: The 3M Company. <https://multimedia.3m.com/mws/media/14303830/3m-filtering-facepiece-shelf-life-letter.pdf>.

3M [2020]. Frequently Asked Questions: 3M Health Care Particulate Respirator and Surgical Masks Storage Conditions and Shelf Life. St. Paul, MN. <http://multimedia.3m.com/mws/media/8692380/3m-health-care-particulate-respirator-and-surgical-masks-storage-conditions-and-shelf-life-faq.pdf>

Alpha ProTech [2019] Alpha ProTech Customer Service Representative, email correspondence, October 1, 2019.

Alpha ProTech [2020] Shelf Life/Expiration Dating. (Appendix 2)

ASTHO [2013]. Federal Emergency Preparedness Directives and Systems- Emergency Authority and Immunity Toolkit. Arlington, VA: Association of State and Territorial Health Officials. <http://www.astho.org/Programs/Preparedness/Public-Health-Emergency-Law/Emergency-Authority-and-Immunity-Toolkit/Federal-Emergency-Preparedness-Directives-and-Systems-Fact-Sheet/>.

Carias C, Rainisch G, Shankar M, Adhikari BB, Swerdlow DL, Bower WA, Pilai SK, Meltzer MI, Koonin LM [2015]. Potential demand for respirators and surgical masks during a hypothetical influenza pandemic in the United States. Clinical Infectious Diseases 60 (1): S42-S51 <https://doi.org/10.1093/cid/civ141>.

DHHS [2012]. An HHS retrospective on the 2009 H1N1 influenza pandemic to advance all hazards preparedness. Washington D.C: U.S. Department of Health and Human Services, <https://www.phe.gov/Preparedness/mcm/h1n1-retrospective/Documents/h1n1-retrospective.pdf>.

Gerson [2019]. Gerson Customer Service, email correspondence, October 1, 2019.

NIOSH [1997]. 42 CFR Part 84 respiratory protective devices. Cincinnati, OH: U.S. Department of Health and Human Services, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, <https://www.cdc.gov/niosh/npptl/topics/respirators/pt84abs2.html>.

NIOSH [2017]. Workplace safety and health topics: healthcare workers. Cincinnati, OH: U.S. Department of Health and Human Services, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, <https://www.cdc.gov/niosh/topics/healthcare/default.html>.

NIOSH [2018]. Standard respirator testing procedures. Cincinnati, OH: U.S. Department of Health and Human Services, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, <https://www.cdc.gov/niosh/npptl/stps/apresp.html>.

NIOSH [2019]. NIOSH conformity assessment notice: NIOSH CA 2019-1012, NIOSH respirator approval contents and meaning. Pittsburgh, PA: U.S. Department of Health and Human Services, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, <https://www.cdc.gov/niosh/npptl/resources/pressrel/letters/conformitynotice/CA-2019-1012.html>.

Patel A, D'Alessandro M, Ireland KJ, Burel WG, Wencil EB, Rasmussen SA [2017]. Personal protective equipment supply chain: lessons learned from recent public health emergency responses. *Health Security*. 15 (3): 244-252
<https://doi.org/10.1089/hs.2016.0129>.

Rottach DR, Lei Z [2017] Stockpiled N95 filtering facepiece respirator polyisoprene strap performance. *J Int Soc Respir Prot.* 34 (2): 69-80 <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC6198819/>.



Frequently Asked Questions: 3M Health Care Particulate Respirator and Surgical Masks Storage Conditions and Shelf Life

Why is 3M adding shelf life information for the 3M™ Health Care Particulate Respirator and Surgical Masks* 1804/1804S, 1860/1860S, 1870, 1870+?

The addition of shelf life information to our 3M NIOSH-approved respirators is a way to communicate to our customers the storage conditions and potential longevity of our respirators. Traditionally the life cycle of these respirators commonly used in health care workplace applications, from date of manufacture to use by the customer, has been short in duration as they are disposable. However, with the increased attention to respirator stockpiling, many customers have requested information on storage conditions and shelf life. We hope that by adding this information to the respirator packaging it will encourage our customers to employ good practices such as appropriate long term storage, rotation of stock and inventory management.

In the United States, per 29 CFR 1910.134, OSHA has required that respirators be stored in the original packaging and away from contaminated areas, dust, sunlight, extreme temperatures, excessive moisture and damaging chemicals. Canada's CSA Standard Z94.4 has a similar requirement.

*Models that are both NIOSH approved N95 filtering facepiece respirators and FDA cleared as a surgical mask.

What 3M Health Care Particulate Respirator and Surgical Masks have a shelf life?

The 3M Health Care Particulate Respirator and Surgical Mask models 1804/1804S, 1860/1860S, 1870, 1870+ have an established 5 year shelf life when respirators are stored in their original packaging within climatic conditions ranging from -4 °F (-20 °C) to +86 °F (+30 °C) and not exceeding 80% RH.

Why does the packaging for some 3M Health Care respirators have shelf life information and other respirator packaging does not?

The transition to updated packaging/labeling in relation to the storage conditions and shelf life has been initiated. However, for a period of time, you may see product packaging in the market place with and without storage condition and shelf life information included/incorporated.

How is the respirator's shelf life communicated?

The shelf life information is usually found on the side or bottom of the primary box. Storage conditions are included in the instructions for use (IFU). The shelf life for the health care NIOSH-approved respirators is in the form of a "use by" date such as "YYYY-MM-DD" (year-month-day) and should be located near the hourglass icon. This information is also located on the label of the shipper case or corrugated box. An explanation of the icons and additional information regarding shelf life and storage conditions can be found in the IFU provided with the respirator. Please refer to the respirator packaging as shelf life is specific to each model.

Here is an example of how storage conditions and shelf life will be depicted in the IFU and primary box respectively (this is an example only):

When stored in original packaging between temperatures from -4 °F (-20 °C) to +86 °F (+30 °C) and not exceeding 80% RH, the respirator may be used until the date specified on packaging located next to the "Use by Date" symbol.

3M Personal Safety Division



Use by Date

Here are some additional symbols that you will see in the updated instructions for use.



Date of Manufacture



Manufacturer's Lot Number relevant to the device bearing the symbol



Manufacturer

What happens if storage conditions are not met?

3M's goal is to help our customers ensure that filtering facepiece respirators stored for extended periods of time will meet the performance requirements to which they were approved and function as intended. When establishing a shelf life, 3M takes into account the filter media as well as the component parts of the respirator such as the strap and any staples. Therefore, we are confident that the respirators will meet performance requirements when the identified conditions are met.

However, when respirators are maintained outside of the established storage conditions, 3M cannot ensure that the respirators will meet performance requirements. In this event, many different kinds of changes can occur to the respirator including cosmetic changes and degradation of components such as headbands, nose foam and noseclips. Examples of cosmetic changes include discoloration of materials. Examples of degradation include crumbling of nose foam or breaking of headbands.

It is always critical that the respirator be inspected and a user seal check be conducted by the wearer per the IFU. If the person wearing the respirator cannot achieve a proper seal the respirator should not be used.

How do we know when not to use the respirator?

First refer to the packaging for a "use by" date. 3M's recommendation is that respirators be disposed of after the stated use by date. Always inspect the respirator and conduct a user seal check before use per the IFU. If the person wearing the respirator cannot achieve a proper seal, then the respirator should not be used. Even for respirators within the stated shelf life, the respirator should be disposed of immediately upon observation of damaged or missing parts. For those respirators that have established shelf life but which packaging is not yet marked with a "use by" date, 3M recommends they no longer be used if 5 years has passed since the date of manufacture.

If the respirator is not marked with shelf life information, how can I determine the age of the respirator?

For respirators that are not currently labeled with shelf life information, the date of manufacture can be determined from the label or printed information located on the primary box as well as the shipper case or corrugated box. For assistance in interpreting the date of manufacture, please call 3M Health Care Helpline at 1-800-228-3957 if in the U.S. In Canada call 1-800-267-4414 Release 5, February 2020. Other countries please contact your local 3M office.

Is it okay to exceed storage conditions and, if so, for how long?

It is recognized that recommended storage conditions may be exceeded for short periods of time during transportation. This has been accounted for in the shelf life determination. However, storage outside the recommended conditions should be avoided when possible.

3M Personal Safety Division

Should the respirator be disposed of after the shelf life has expired?

3M's recommendation is that the respirator be disposed of after the stated use by date has expired.

Will 3M take back respirators that have reached the end of their stated shelf life?

No, 3M will not accept returns of respirators on the basis of shelf life.

Will all 3M respirators have the same shelf-life?

No, not all 3M respirators will have the same shelf life. In making shelf life determinations, 3M takes into account the filter media as well as the components of the respirator. Components vary from model to model. See the [3M Filtering Facepiece Shelf Life](#) document for model specific information.

Personal Safety Division
3M Center, Building 235-2W-70
St. Paul, MN 55144-1000

3M PSD products are
occupational use only.

In United States of America
Technical Service: 1-800-243-4630
Customer Service: 1-800-328-1667
3M.com/workersafety
In Canada
Technical Service: 1-800-267-4414
Customer Service: 1-800-364-3577
3M.ca/Safety

© 3M 2020. All rights reserved.
3M is a trademark of 3M Company and
its affiliates.
Used under license in Canada.
All other trademarks are property
of their respective owners.
Please recycle.
Release 5, February 2020



AlphaProTech

236 North 2200 West
Salt Lake, UT 84116
Office: 801-355-5816
Fax: 801-355-2534
www.alphaprotech.com

January 30, 2020

Shelf Life / Expiration Dating

This letter is in response to an inquiry on the requirement to label medical devices with an expiration date/shelf life. In accordance with the Food and Drug Administration (FDA) and guidance pertaining to this issue, shelf life dating solely for package integrity and sterility is not typically required. Expiration dating may be needed only if the device components contain a finite useful timeframe. Views in the industry see expiration dating as a safety factor and shelf life as a quality factor. While FDA interprets these items in a similar nature their view as to need of such date on packaging arises from the intended product make-up having limiting usefulness, degrading of components, or undesired package product interactions. With this being said, AlphaProTech (APT) does not include, as part of labeling, or related insert material, information pertaining to shelf life or expiration dates on their product lines due to the FDA guidance.

While APT's product lines do not specifically contain printed shelf life/expiration dates, defined testing on older products reveals these products continue to exceed the minimum requirements. Degradation of quality or safety on older product has not been seen in laboratory tests. Literature or labeling dealing with shelf life/expiration dating may be incorporated at a future date.

Please allow this memo to assist in clarifying any concerns you may have had about APT's exceptional products. If additional information or clarification on this subject is needed, please feel free to contact me.

Kind Regards,



Eric T. Llewelyn
V.P. Quality & Regulatory Affairs
Phone: (801) 355-5816
www.alphaprotech.com

