NPPTL COVID-19 Response: International Respirator Assessment

Manufacturer: UNKNOWN, (Makrite Industries, Inc.)

Model Tested: 9500-N95; Lot# 062420

Date Tested: October 6, 2020

These findings pertain to the UNKNOWN, (Makrite Industries, Inc.), model 9500-N95; Lot# 062420. The packaging and labeling indicate that it is a NIOSH-approved product, under approval number TC-84A-5411. The packaging also indicates that it meets GB2626-2006 (the Chinese standard for Respiratory Protective Equipment – Non-Powered Air-Purifying Particle Respirator). "UNKNOWN" has been listed as part of the manufacturer name since the packaging box lists "Dongguan Sure-On Industrial, Ltd.", but a packaging sheet lists "Dongguan Sure-On Plastic & Fiber Products Co., Ltd.". (See pictures at the end of this report).

Ten respirators were submitted for evaluation. The samples were tested using a modified version of NIOSH Standard Test Procedure (STP) TEB-APR-STP-0059. This modified assessment plan can be found here.

The maximum and minimum filter efficiency was 99.72% and 99.43%, respectively. All ten respirators measured more than 95%.

This product has head bands/straps. While filter efficiency shows how well the filter media performs, users must ensure a proper fit is achieved.

This assessment is not a part of the NIOSH respirator approval process and will in no way lead to or preclude NIOSH approval through the official approval process. This assessment was developed as an assessment of the filter efficiency for those respirators represented as certified by an international certification authority, other than NIOSH, to support the availability of respiratory protection to US healthcare workers due to the respirator shortage associated with COVID-19. Only particulate filter efficiency was assessed.

The results provided in this letter are specific to the subset of samples that were provided to NPPTL for evaluation.

These results will be used to update the CDC guidance for <u>Crisis Capacity Strategies</u> (during known shortages).

Evaluation of International Respirators



Pictures have been added to the

end of this report.

Test: Modified TEB-APR-STP-0059

Date Tested: October 6, 2020

Report Prepared: October 7, 2020

Manufacturer: UNKNOWN, (Makrite Industries, Inc.)

Item Tested: 9500-N95; Lot#062420

Country of Certification: China (GB2626), USA (claimed, 42 CFR 84)

Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH₂O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency (%)
1	85	14.3	0.41	0.41	99.59
2	85	14.4	0.51	0.51	99.49
3	85	14.4	0.40	0.40	99.60
4	85	16.4	0.39	0.39	99.61
5	85	15.5	0.56	0.56	99.44
6	85	16.7	0.37	0.37	99.63
7	85	14.4	0.57	0.57	99.43
8	85	16.6	0.28	0.28	99.72
9	85	13.5	0.51	0.51	99.49
10	85	14.9	0.44	0.44	99.56
P	Minimum Filter Effi	ciency: 99.43%	Maximum Filter Efficiency: 99.72%		

- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of
 respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and
 therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.






RESPIRATOR FITTING INSTRUCTION Hold the respirator in hand with the nosepiece at your fingertips, allowing the headbands to hang freely below STEP 2 Press the respirator firmly against your face with the nosepiece on the bridge of your nose. STEP 3 Stretch and position the top band high on the back of the head. Stretch the bottom band over the head and position below your ears. STEP 4 Using both hands, mold nosepiece to the shape of your nose. STEP 5 To test fit: a) Cup both hands over the respirator being careful not to distrub position, and b) inhale vigorously. If air leaks around the edges, reposition the straps or adjust strap tension for better fit. Please carefully follow these fitting instructions during each use to achieve proper fit. MAKRITE INDUSTRIES INC. 11F-5, No. 79, Sec 1, Xintai 5th Rd., XiZhi Dist, New Taipei City 221, Taiwan Telephone: 886 2 2698 2419 Manufactured by Dongguan Sure-On Industrial Ltd. No.18, Guangyuan St., 168 Industrial Area, Zho Fo Ling, Tang Xia, Dongguan City, China Telephone: 0769-87723170 www.makrite.com





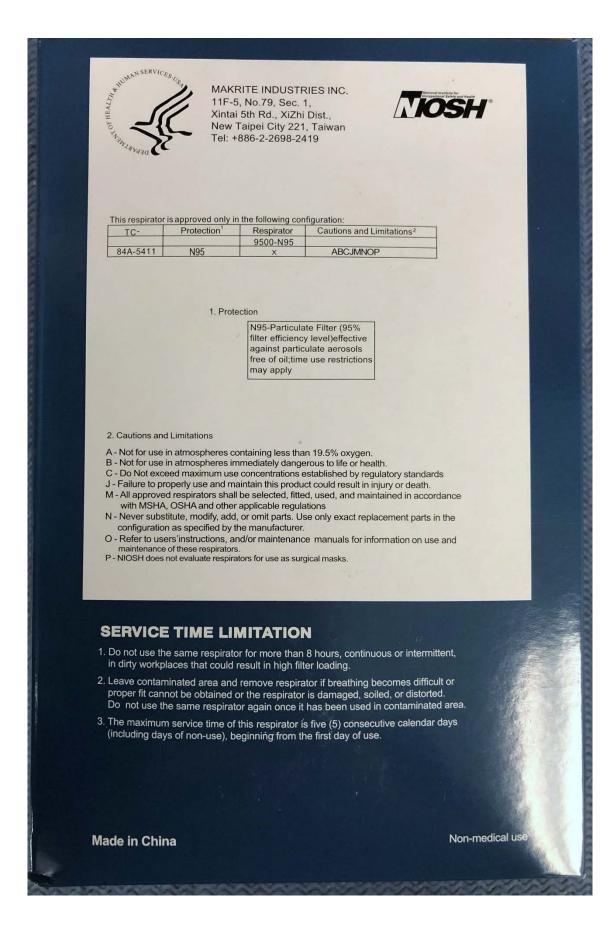







NPPTL COVID-19 Response: International Respirator Assessment





